

DYNAMIC
ABUTMENT®
SOLUTIONS

CAD-CAM
solutions



DYNAMIC ABUTMENT® SOLUTIONS

ALCALDE MONTANYA, 17 · 25005 · LLEIDA (SPAIN)
INTERNATIONAL +34 973 289 580
das@dynamicabutment.com

SPAIN +34 973 289 580
spain@dynamicabutment.com

Dynamic Abutment® Solutions is the trademark of the manufacturer Talladium España S.L.

The information included in this catalogue is exclusively addressed to professionals in dental sector.

All commercial trademarks mentioned herein are fully registered by their respective companies, and the images that appear are just to provide an orientation.

Talladium reserves the right to modify this document without previous notice.

Talladium is not responsible for the inadequate execution of these products if the warning indications corresponding to every reference are not contemplated.

All of the products listed in this brochure are marking in accordance with CE legislation. Some of the products are not authorized for sale and distribution or do not have a sales license in some countries according to other legislations (FDA, CMDCAS, etc.) Please ask for information: das@dynamicabutment.com



Marking in accordance with CE legislation and applicable sanitary regulations



Visit our Online Store to find all our products and compatibilities :

www.dynamicabutmentstore.com

4	DYNAMIC ABUTMENT® SOLUTIONS
5	RESEARCH & DEVELOPMENT
6	QUALITY CENTER
7	INTERNATIONAL CUSTOMER SERVICE
8	DYNAMIC SYSTEM
10	DYNAMIC SYSTEM FOR MILLING STRUCTURES
12	CADCAM WORKFLOW - DAS PRODUCTS
14	DYNAMIC µSCANBODY/ADAPTOR
16	LAB SCANBODY
17	SCANALOG
18	DYNAMIC TIBASE®/DYNAMIC 3TIBASE®
20	DYNAMIC TIBASE® GINGIVAL OPTIONS
22	DYNAMIC PREMILL3D®/ADAPTORS
24	DYNAMIC MILLING TOOL - DMTONE®
26	DIGITAL ANALOG
28	DAS LIBRARIES
30	DAS CUSTOMIZED SERVICES
32	CAD-CAM
36	DYNAMIC SYSTEM - LIST OF COMPATIBILITES
52	DYNAMIC SYSTEM COMPATIBILITES
162	DYNAMIC SCREWS TECHNICAL SPECIFICATIONS
165	DYNAMIC SCREWDRIVER & DYNAMIC SCREWS
166	STRAIGHT SCREWS TECHNICAL SPECIFICATIONS
169	SCREWDRIVERS & STRAIGHT SCREWS
170	INTRAORAL SYSTEM COLORS ACCORDING TO COMPATIBILITY
174	DYNAMIC MILLING TOOL SPECIFICATIONS
176	SCREWDRIVER ADAPTOR/COMPLEMENTS
177	IDENTIFICATION PRODUCT/ SECURITY & TRACEABILITY
178	TALLIUM GUARANTEE

THE ART OF CHANGE

The dental sector has evolved more in recent years than in the last four decades. The arrival of digitalisation now reverberates through all laboratory and dental clinic work processes. This process brings with it new workflows and new tools to be used in the process.

The premise of “adapt or die” is a reality. And that is why research and innovation has enabled us to be at the forefront of sector digitalisation and first to provide our clients and associates with innovative technological solutions.

Since our founding over 15 years ago, we have been a revolutionary force in the dental sector, rejigging preconceived ideas of workflows, angled solutions and dental aesthetics. This is the art of change. Of doing something before anyone else. Of being dynamic.

The dental sector will continue to evolve and new work processes will arise. And, of course, Dynamic Abutment® Solutions will be at the cutting edge and the first to offer comprehensive solutions to these changes. This is the art of innovation, of revolution. This is **the art of CHANGE**.

“Focus on excellence and R&D&I has seen us become No.1 in angled solutions”

The R&D&I Department at Dynamic Abutment® Solutions is endorsed by the UNE 166002 certificate for R&D&I systems management.

It is actively involved in international projects, working alongside the main operators in the sector, contributing know-how in both production and machining and the design of digital hardware for CAD and production management (CAM).

Consequent to this work with the leading figures and companies in the sector, we develop new products that are rolled out from our own Production Center. The Production Center features next-gen equipment, enabling us to make prototypes prior to receiving the final thumbs-up for the product from the R&D&I Department.

The R&D&I Center ensures comprehensive control over all the development stages for new projects, allowing them to be transformed into new products featuring the top-notch safety and quality levels that characterise our output and reaching our clients as soon as possible.



QUALITY CENTER

“Controlling our quality process ensures the safety of our products”

Dynamic Abutment® Solutions has a Quality Center with the very latest metrology and control, prototyping and physical-chemical treatment equipment, and sanitary areas for refitting and packaging health products in an ISO-8 clean room.

Controlling the whole quality process ensures that our products are measured, inspected and checked using the most advanced control methods in the sector. We guarantee the quality of our products from production all the way through to packaging.

Being present in international markets means we have the mandatory health certificates that cover our product:



CE marking, CMD/CAS regulations, or FDA certificates, among others.

Our primary concern from the very beginning has been the quality and safety of our products: UNE-EN ISO 9001:2015, UNE-EN ISO 13485:2016, and UNE 166002:2014.

INTERNACIONAL CUSTOMER CENTER

“Our experience and know-how serving our clients and distributors”

The main objective of the exclusive Dynamic Abutment® Solutions Customer Service Center is to maintain a constant channel of communication with our distributors and associates.

Our products are available in over 45 countries across five continents, with guaranteed health product management and certificates for international markets.




We offer our clients technical support, along with immediate answers and solutions with direct support from the R&D&I technical department for even the most complex of cases.

We participate in fairs, events, conferences and training sessions through our distributors and associates.



Direct contact with and suggestions from our clients allows us to continue improving the quality of the products and services we offer.

DYNAMIC SYSTEM

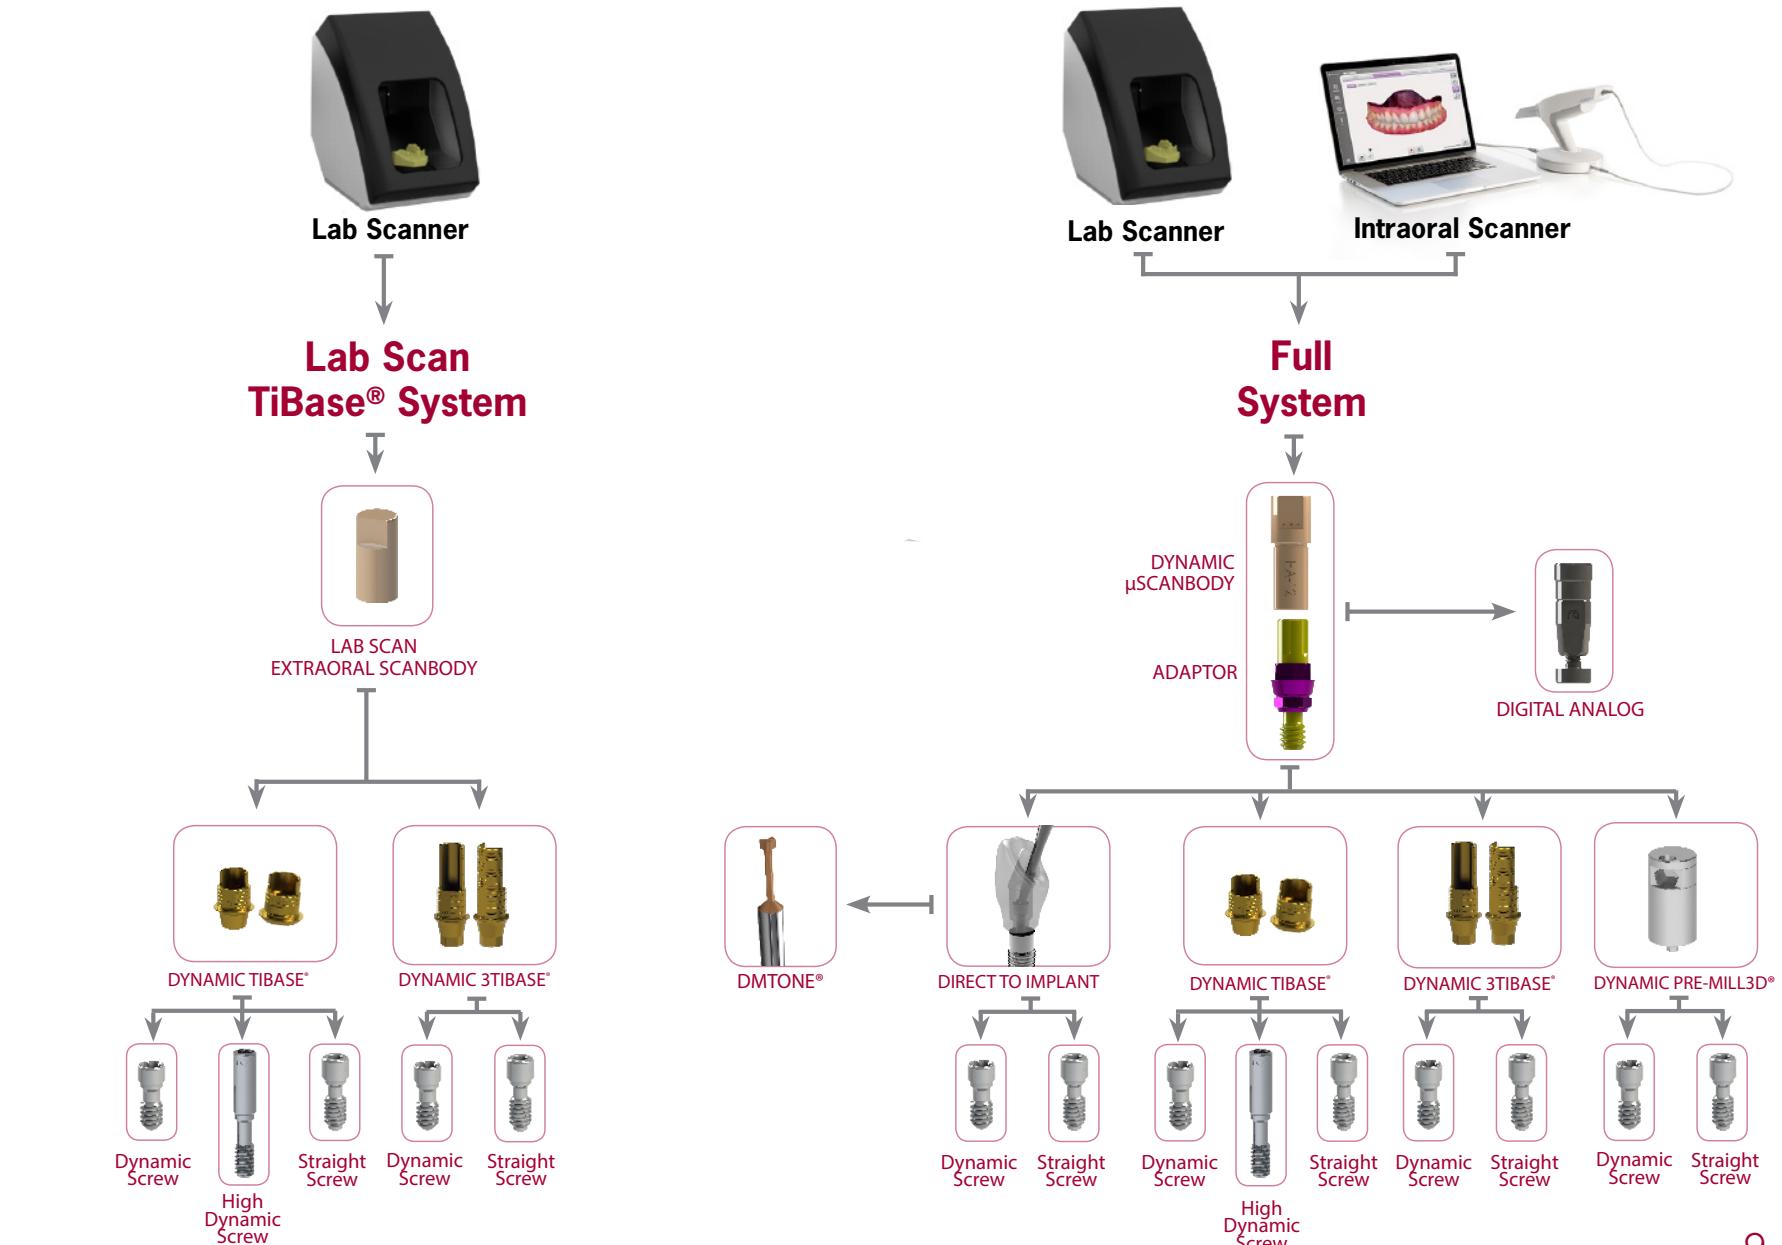

DYNAMIC SYSTEM for MILLING STRUCTURES

The Screwdriver set of 3.0 Dynamic Abutment® System is used in those cases in which rectification of the entry of the screw due to an unfavorable position of the implants is necessary, improving the functionality and aesthetics of the milled prosthesis.

More than 500.000 cases resolved with
DYNAMIC SYSTEM




PATENT NUMBER
Dynamic Screwdriver
EP 3 260 079

Dynamic Screwdriver

Screwdriver with hexalobular head, exclusively to the 3.0 Dynamic Abutment® system.

Lengths: 18, 24, 32mm.

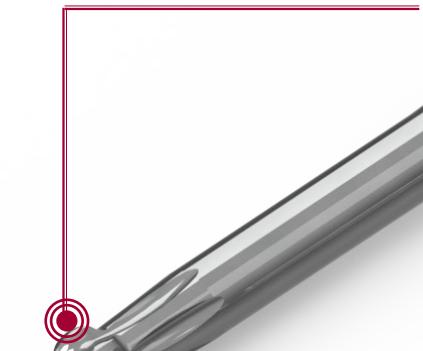

PATENT NUMBER
Dynamic Screw
EP 2 932 937

Dynamic Screw

Dynamic screws cover the majority of the thread metrics available on the market. They are used with the Dynamic TiBase® or milled structures with an angled screw channel. There are several lengths for each metric to ease adaptation to the structures. All of them are made of Titanium grade V.



Our screwdriver has a contra-angle connection to make it easier to use with a dynamometer or manual ratchet, with the corresponding adaptors or handles.

High Dynamic Screw

All screws are perfectly identified with their batch and reference numbers, which allow each and every screw to be traced and recorded in the patient's card and in the clinical or laboratory records. Only the 3.0 dynamic screwdriver must be used to install them.

DAS PRODUCTS

CAD-CAM WORKFLOW



DYNAMIC μ SCANBODY


The scanbody detects the position and orientation of the respective dental implant or analog in CAD-CAM scanning procedures.



Hole free scanbody and not screwed

There are no holes in the upper section which means the Z axis is free to improve scanbody scanning.

The angulation of the chimney it goes always on the opposite side of the scanbody lateral cut.

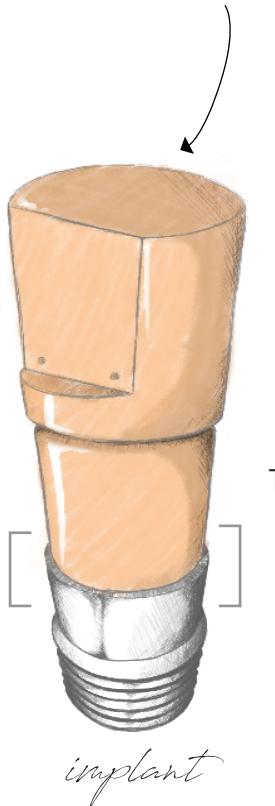

The diameter of the scanbody is always equal or smaller than the implant diameter.

3 lenghts

(8mm, 10mm and 12mm) for the most complex scanbody reading cases.

ADAPTOR

Fastened to an adaptor using a magnet



OPTION 1

library
DAS_I_XXXX


OPTION 2

library*
DAS_IG_XXXX

*Use IG Library code
with the 3mm adaptor

Connecting element between the scanbody and the implant. Marked with different colors according to the compatibility.*

*See pages 170 to 173

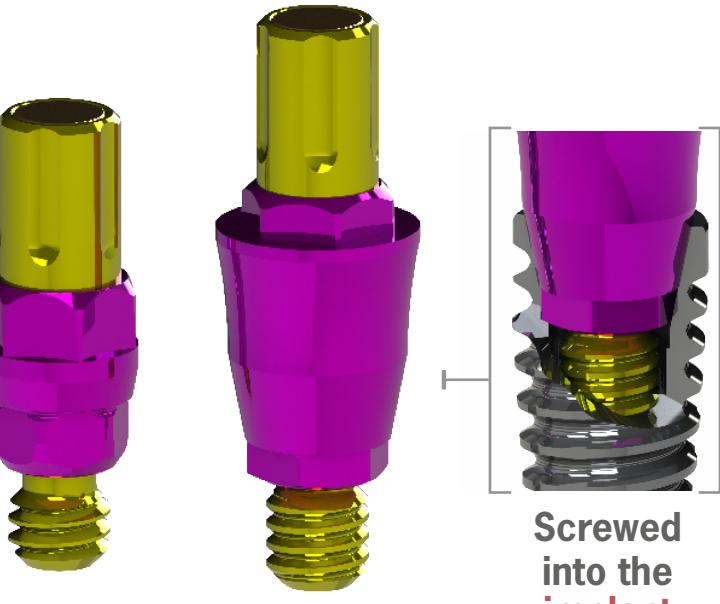



Special screwdriver
for the adaptor*

*See page 176




LAB SCANBODY

Only for Dynamic TiBase®
and Lab Scanner

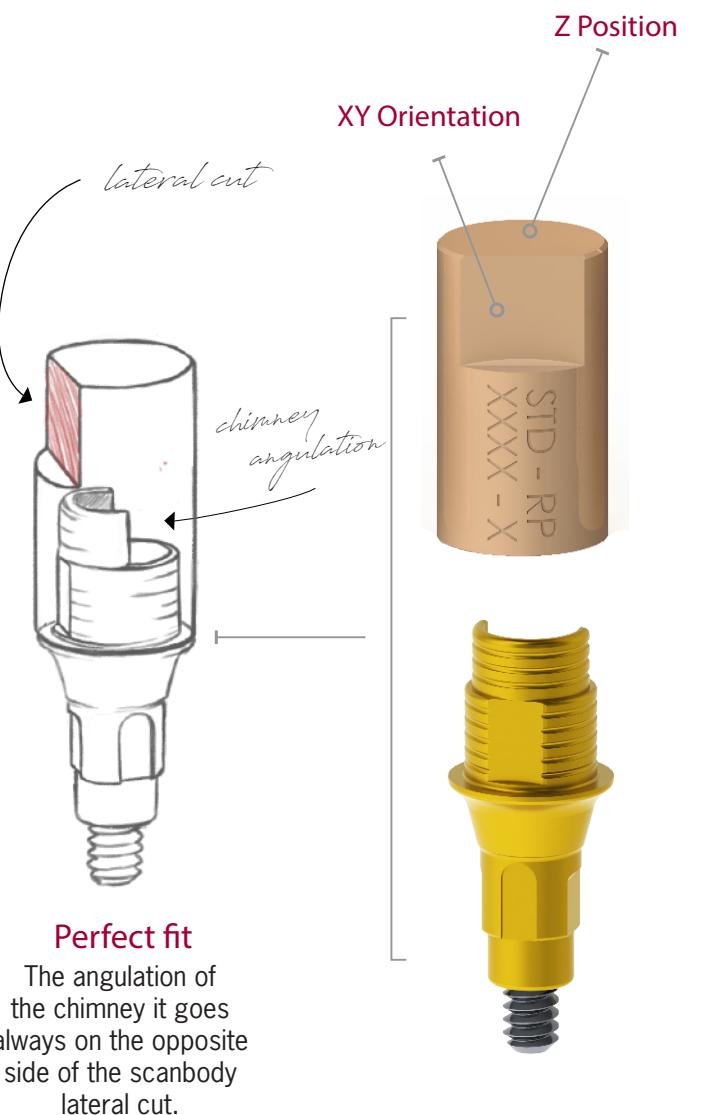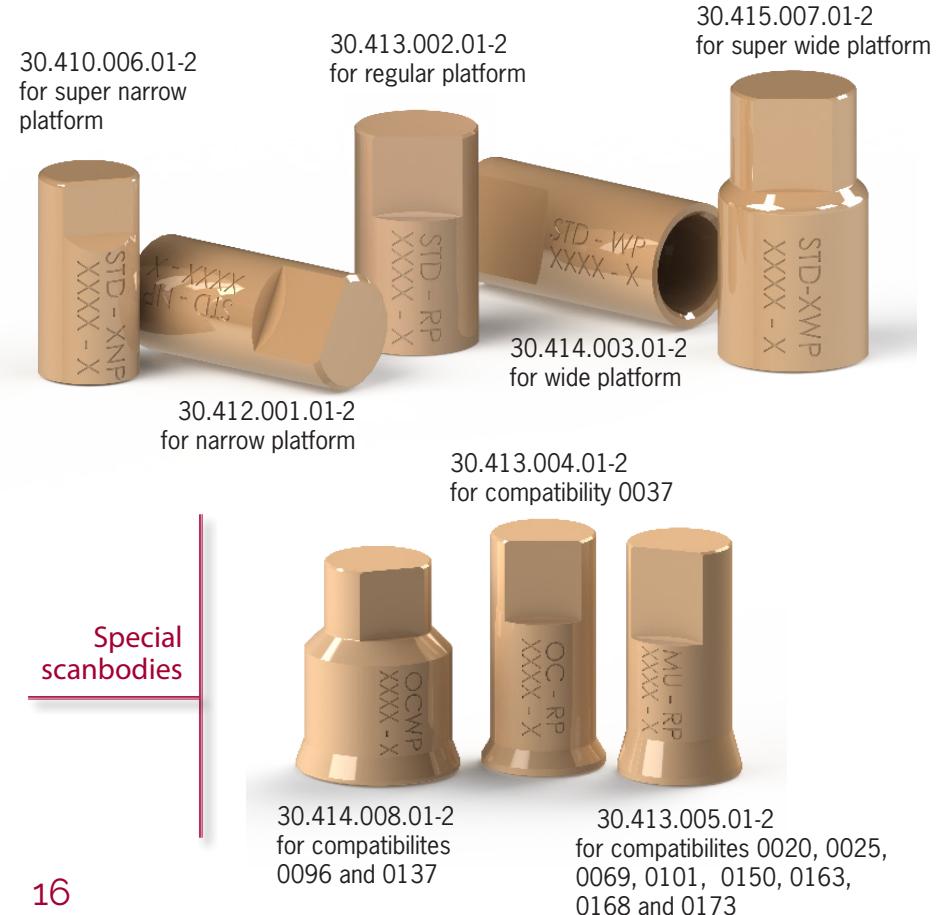

ScAnalog

Scan directly on the impresion tray

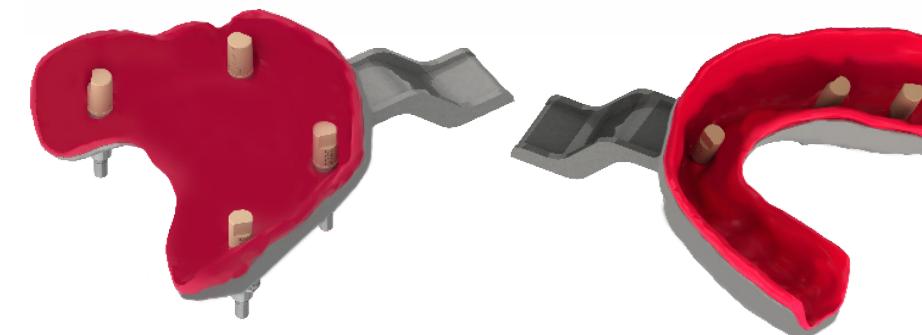

Scanning

Scanning process of the silicon model with the ScAnalogs placed.


DYNAMIC TiBASE®*

Dynamic TiBases® are a technological contribution to the digital treatment for the angled systems development using CAD-CAM: the Dynamic System includes the Dynamic TiBase®, the dynamic screw-screwdriver set, scanbodies and digital libraries available for the main CAD softwares on the market: Exocad, 3Shape, Dentalwings and Dental Cad.

PATENT NUMBER
Dynamic TiBase®
US 10.130.447

TO CORRECT ANGULATION

up to
45°

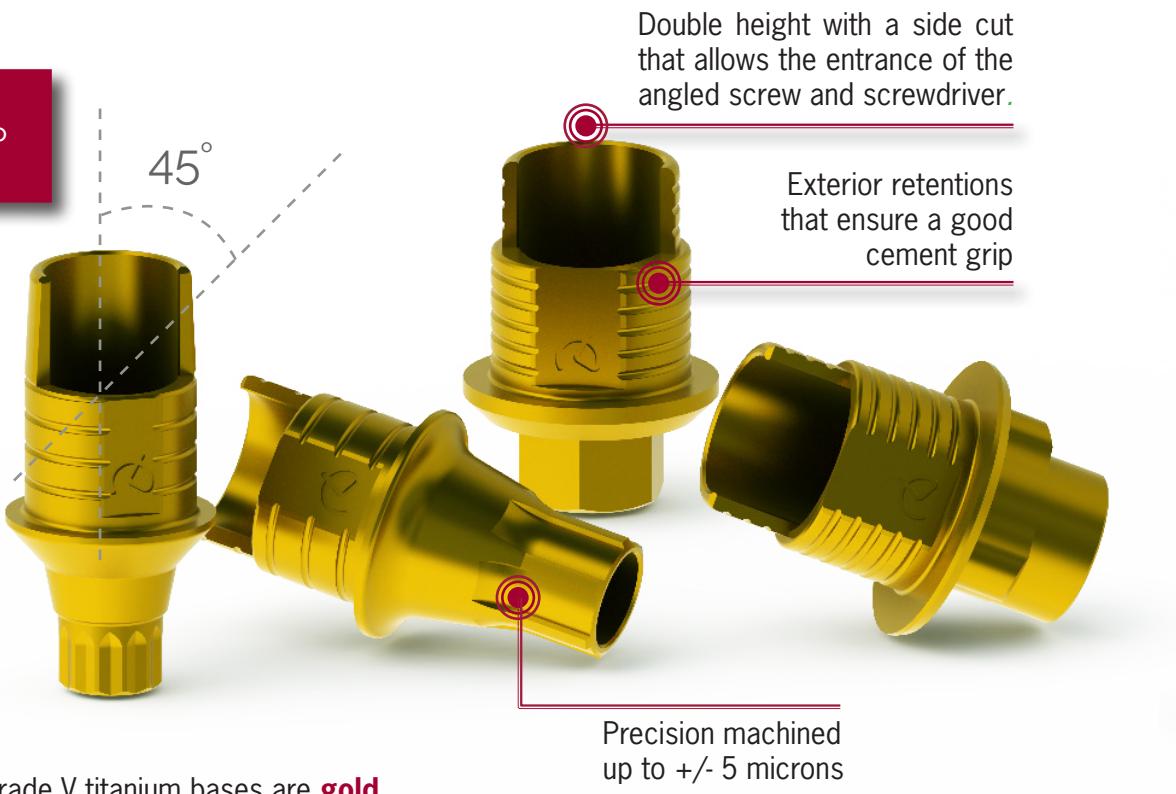


*Maximum angulation available for the first TiBase gingival height.
Maximum angulations for the rest of gingival heights under development

Our grade V titanium bases are **gold anodized** to improve the work's aesthetic.

DYNAMIC 3TiBASE®


The Dynamic 3TiBase® offers the possibility to work with different cement heights: 5, 7 or 9mm. It is specially designed for the cases that require higher height. In this way, a greater support surface is achieved, the structure is stronger and more resistant so structure breaks by height decompensation between the TiBase and the structure are avoided.

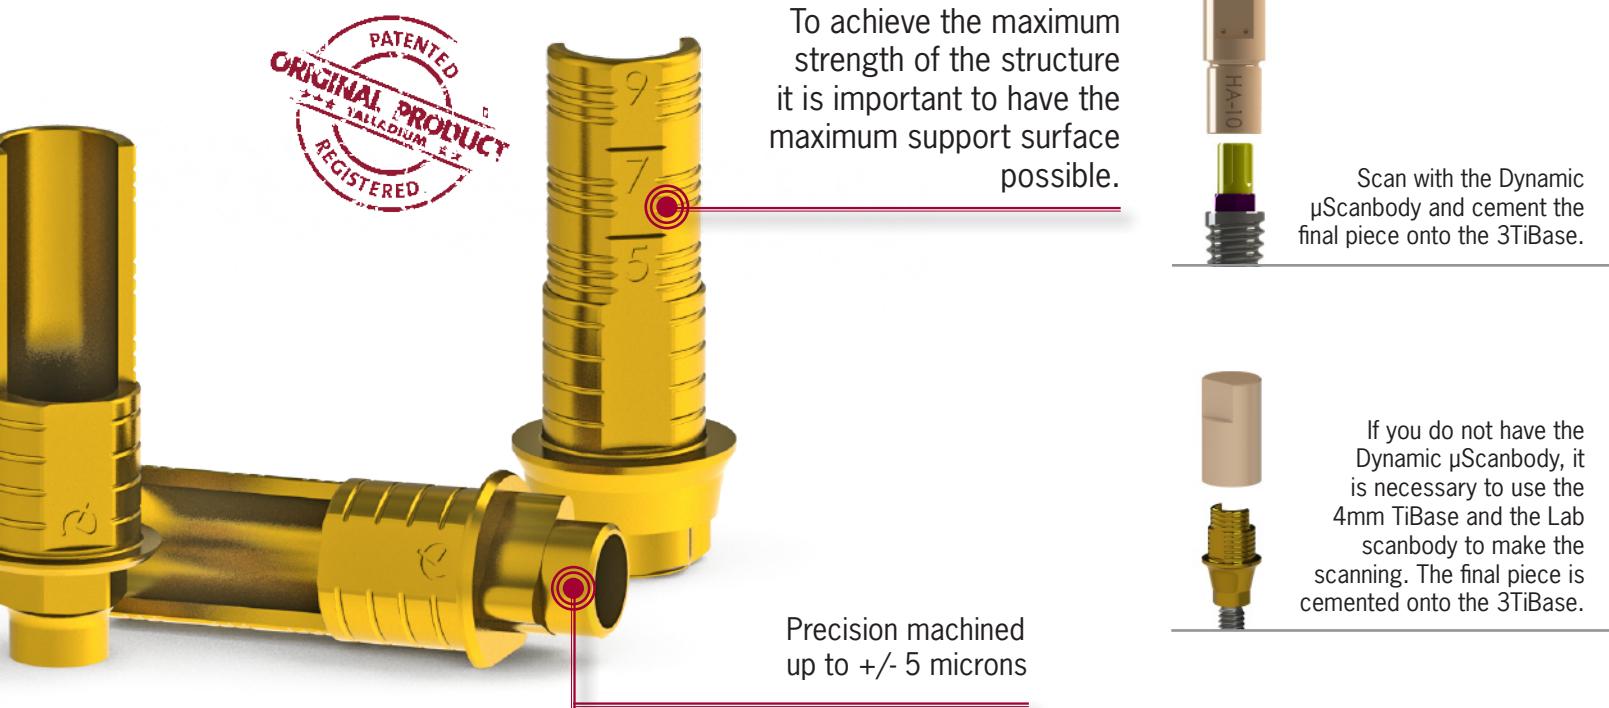

If you do not have the Dynamic μScanbody, it is necessary to use the 4mm TiBase and the Lab scanbody to make the scanning. The final piece is cemented onto the 3TiBase.

DYNAMIC TIBASE®

Gingival options

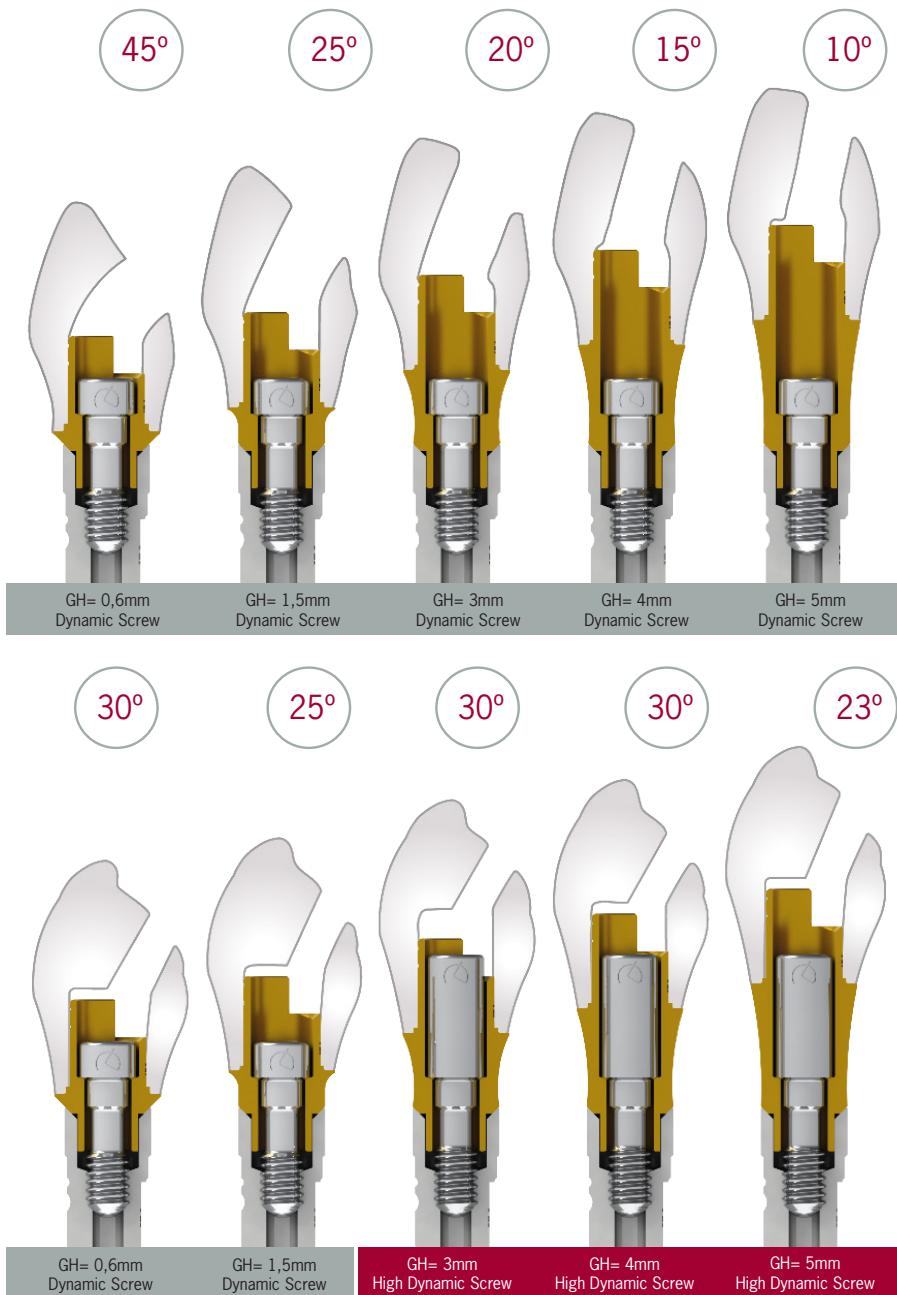

*Example with TiBase® compatible with
Zimmer Screw-Vent Ø3,5 (Code 0040)



STANDARD SYSTEM*



CAPTIVE SYSTEM*


- ✿ Keep the angulation
- ✿ Best aesthetic angled channel Ø 2mm
- ✿ Angled channel reduction of 32%
- ✿ Increases the volume of the structure
- ✿ Captive Screw

(Put the screw on the TiBase® before cementing)




22

DYNAMIC PRE-MILL 3D®



Pre-milled angled channel

The Dynamic Premill3d® already comes with a pre-milling of the inner channel



Angulation from 0 to 30° choice

Allows to choose angulation of the screw channel on the CAD for the later insertion of the screw




Milling of the angulated screw channel

CAD design and milling of the angled channel on CAM by the customer



Dynamic Pre-milled final structure

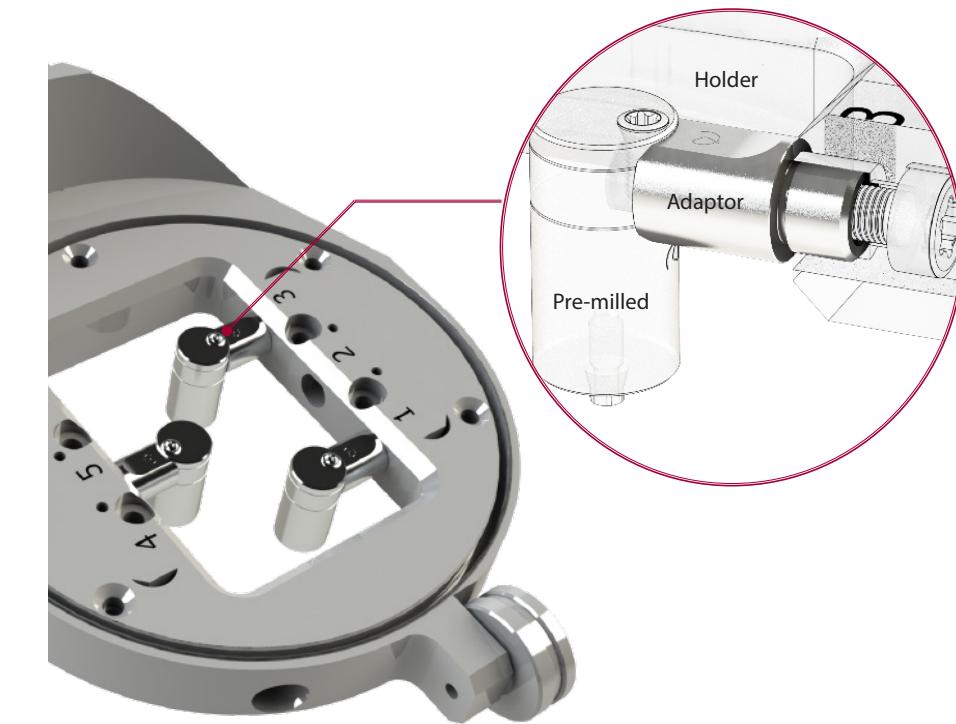

ADAPTORS



Ref: 39.903.001.01-2




Ref: 39.903.002.01-2



Ref: 39.903.003.01-2



Ref: 39.903.008.01-2

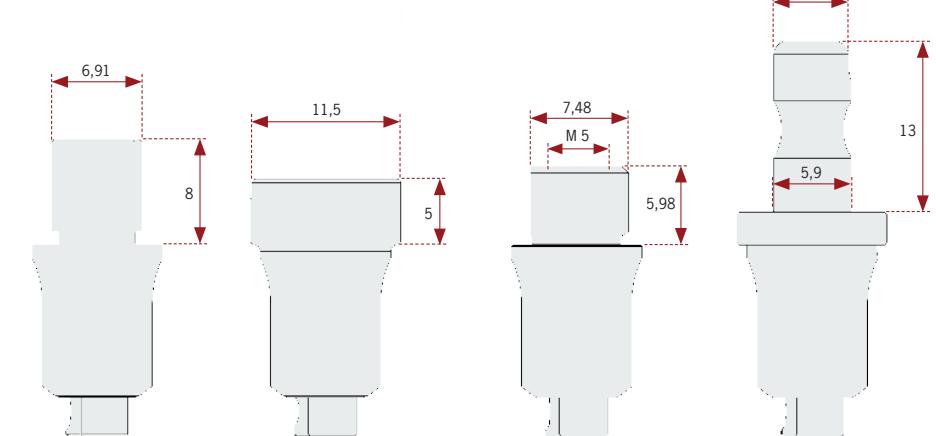

Customized ADAPTORS

We design and manufacture the adapter for any type of holder
das@dynamicabutment.com

23

DYNAMIC MILLING TOOL

Each tool is compatible depending on screw seating, metric and length




Shank
Ø3, Ø4, Ø6

DMTONE
DYNAMIC MILLING TOOL


DIRECT TO IMPLANT (one piece) and ANGULATED

Precision milling tool. In the screwed angled structure direct to implant, it is used to mill the screw seating and to increase the internal diameter of the straight channel.

There are 3 cutting wing-tips with 3 different cutting area each, to mill the screw seating and to increase the internal diameter of the straight channel.

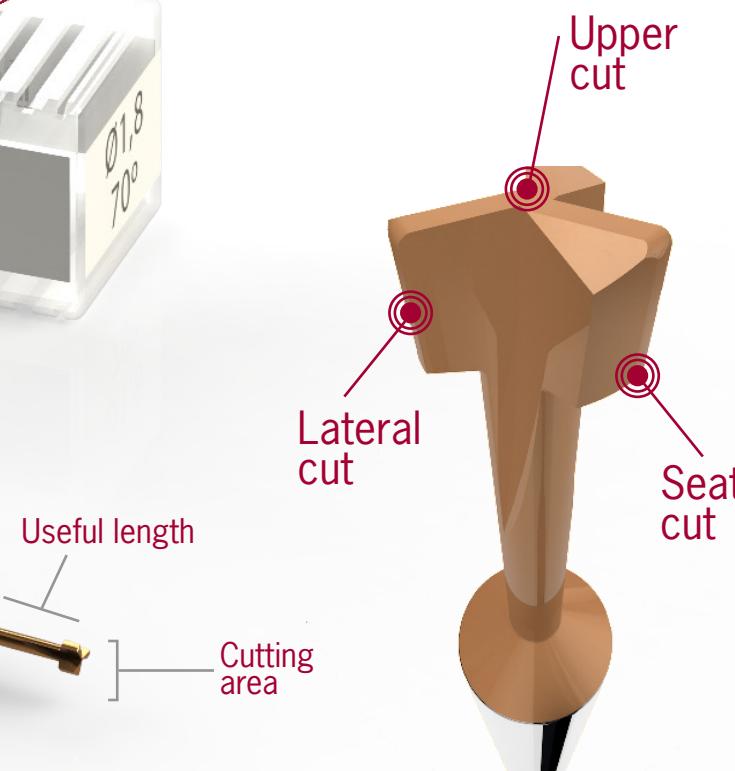


PATENT NUMBER
Milling process of the
angulated channel
ES 2658 985



STEP 1:
Crown with
pre drill.




STEP 2:
Crown with
Angled channel.

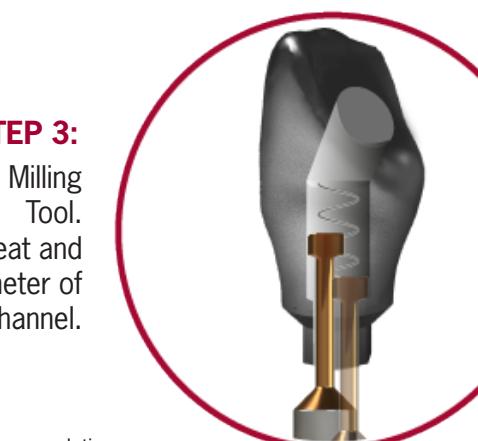


STEP 3:
Crown with Dynamic Milling Tool.
Milling the screw seat and
increasing the diameter of
the straight channel.

*Direct to implant maximum angulation
under development

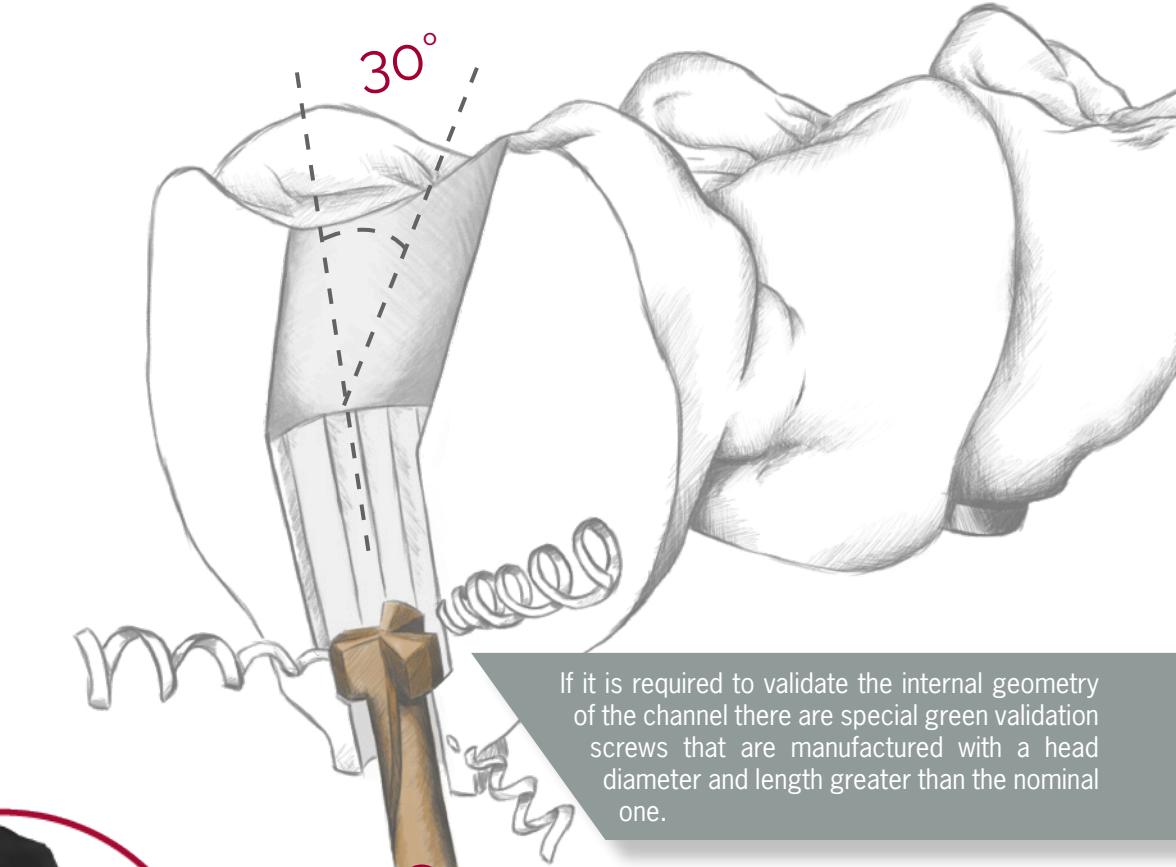


**TESTED and
VALIDATED by**



DIGITAL ANALOG

Digital analog of the dental implant to simulate implant position in a 3D printed dental model.




3 D PRINTED MODEL

The dental model - for later insertion of the analogs - is designed using the CAD libraries.




Concave notch

Top precision in longitudinal position

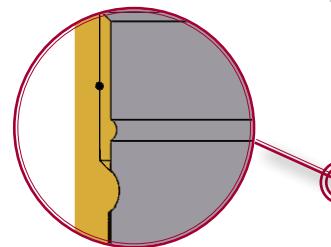


Curved Surface

Accuracy of orientation guaranteed


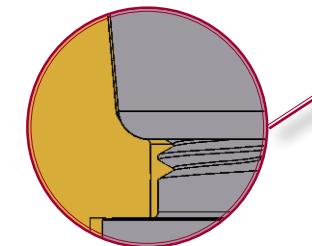


Longitudinal cut

Longitudinal cut to avoid rotation X-Y



DAS LIBRARIES


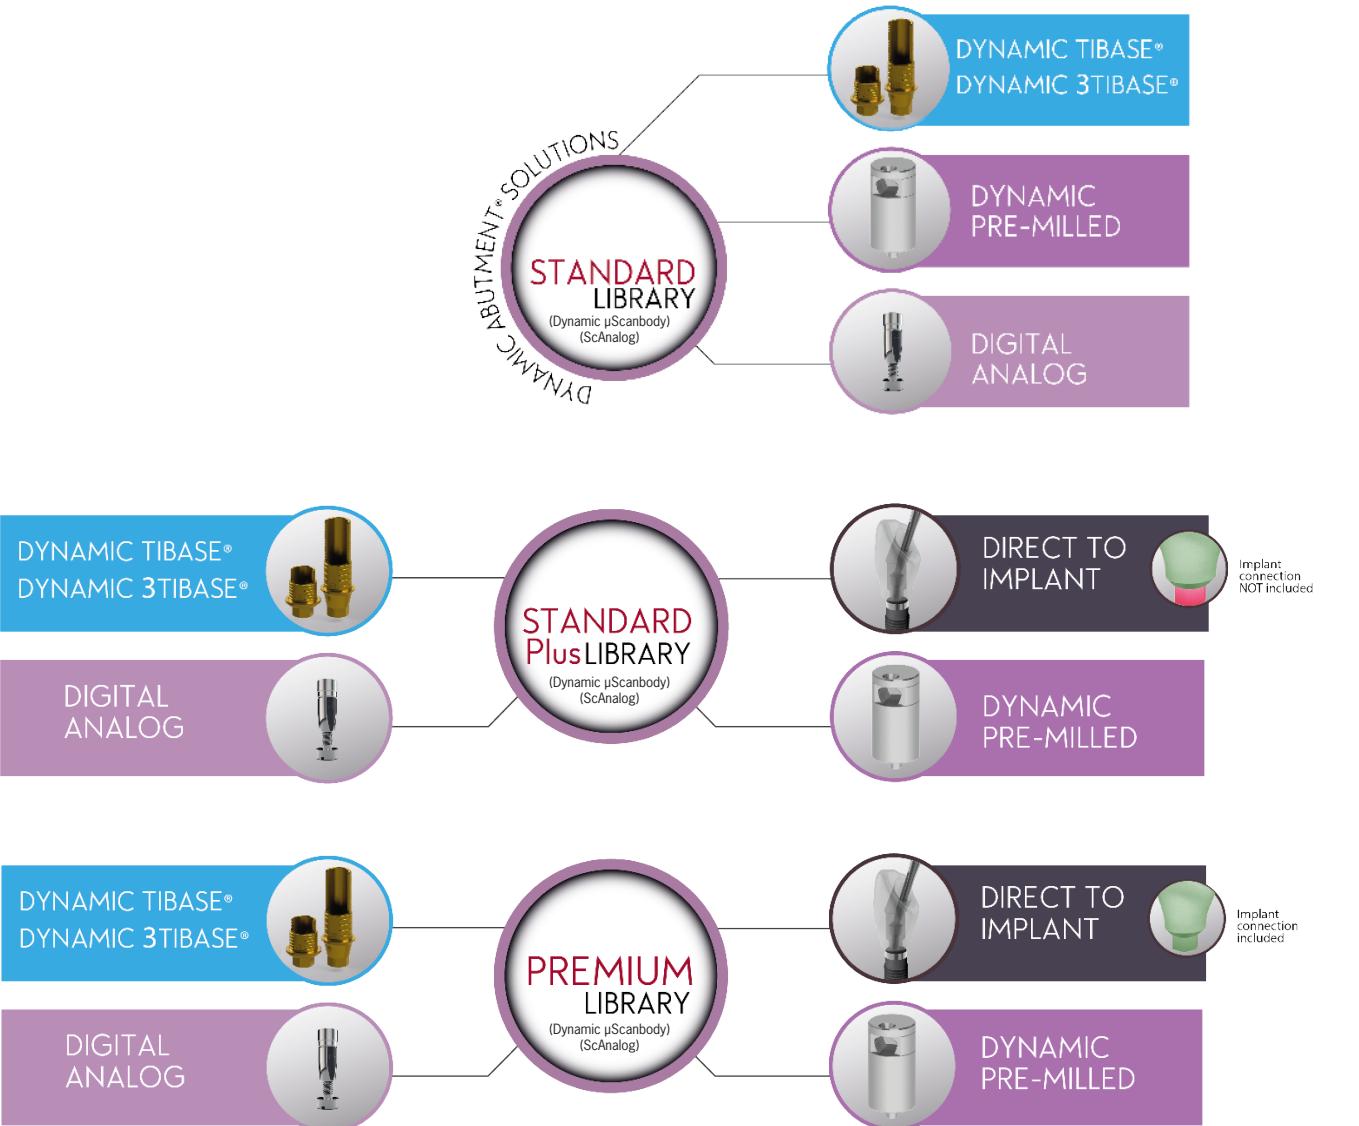
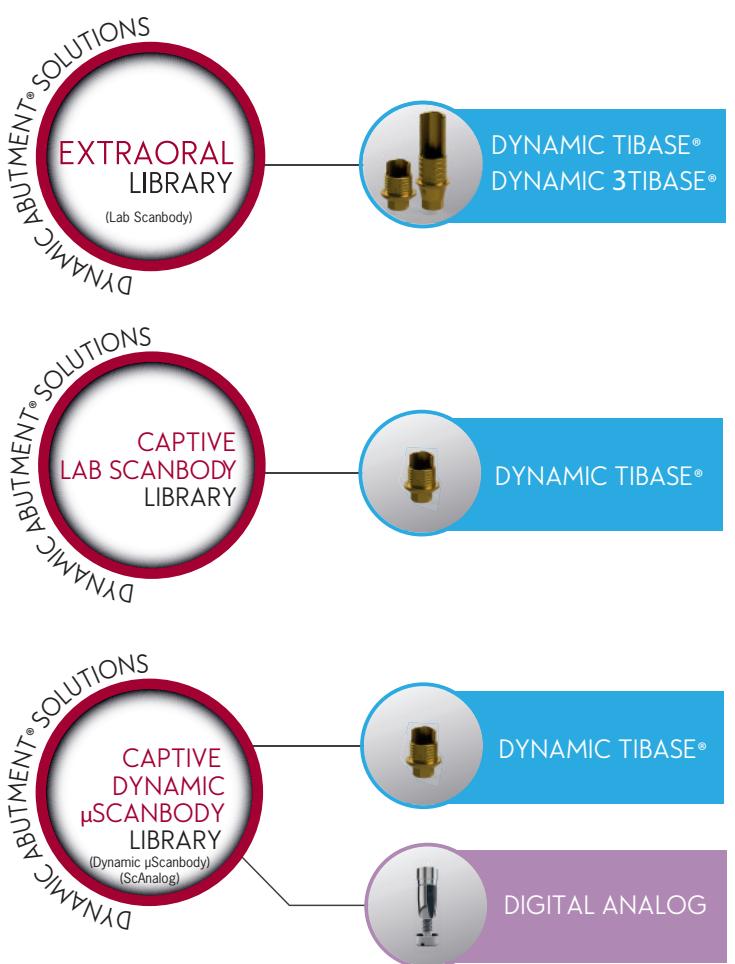


DAS CUSTOMIZE SERVICES

PRODUCT DEVELOPMENT


Any DAS traded goods can be made-to-measure or adapted to your work protocol. DAS complements the development of new products with the technological support (software, libraries, tools, etc.) necessary, alongside all the guarantees any healthcare product needs.

CAD ADAPTION SERVICES



- Adjustment of the CAD libraries for our products to client needs: angled channel diameter modification, calibration of cemented gap TiBase®, adjustment of 3D digital analog printing gap, etc.
- CAD libraries supplied with implant connections; DAS currently has over 500 implant compatibilities.
- Development of special CAD libraries for connections pertaining to the client.
- Design of libraries linked to client's specific scanbodies.
- Etc.

CAM SUPPORT and ADVICE

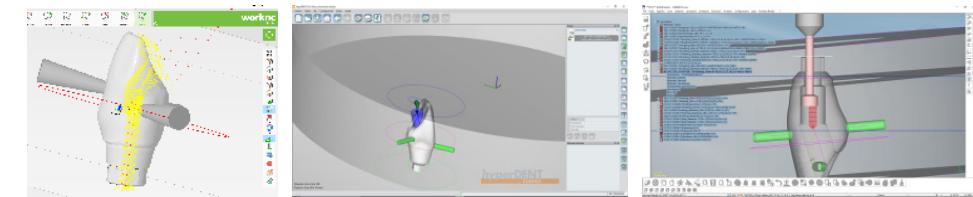

Dynamic Abutment® Solutions products have been tested and validated by the leading CAM software brands on the market.

- Provision of implant connections with nominal values.
- Design and production of special tools to mill connections or special geometries (abutments).
- Design and production of special supports for your milling equipment: pre-milled supports, etc.
- Technology for machining angled channels (copyright-free).


SPECIALIZED CONSULTANCY




Multidisciplinary experience in different areas of dental research and regular collaboration on projects with the key operators in the sector have provided us with experience and know-how that we want to make available to you, so we can advise you, work together and pursue customized projects.
All DAS technological and human resources are available to help turn your idea into a reality, providing expert advice and support throughout all the developmental stages.

DYNAMIC TIBASE®


CAD

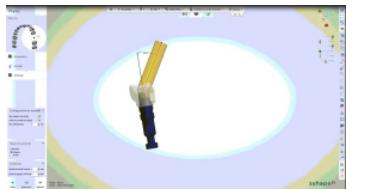


3shape ▶

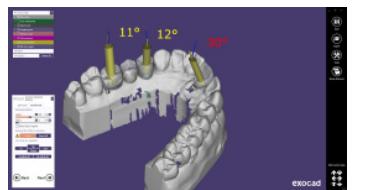

exocad




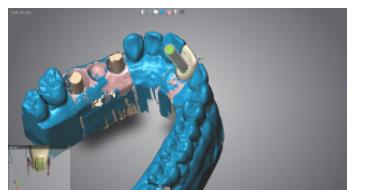


dental wings

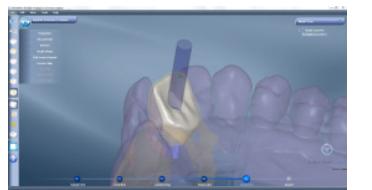

DentalCad

CAM

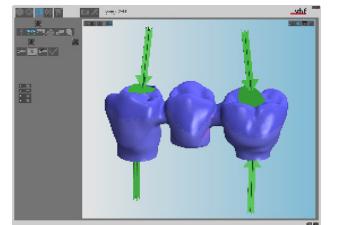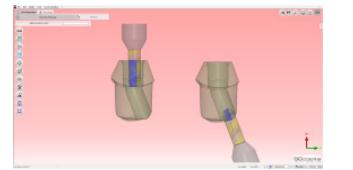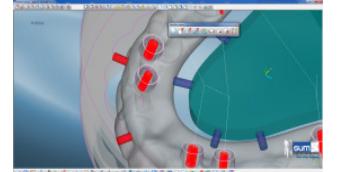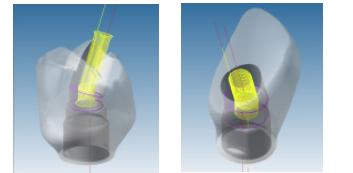

Tested CAM
Software

worknc
Dental


→ FOLLOW-ME I
TECHNOLOGY GROUP

MILL
BOX | sum3D


GO2dental
cam for dental labs

vhf

DIRECT to
IMPLANT

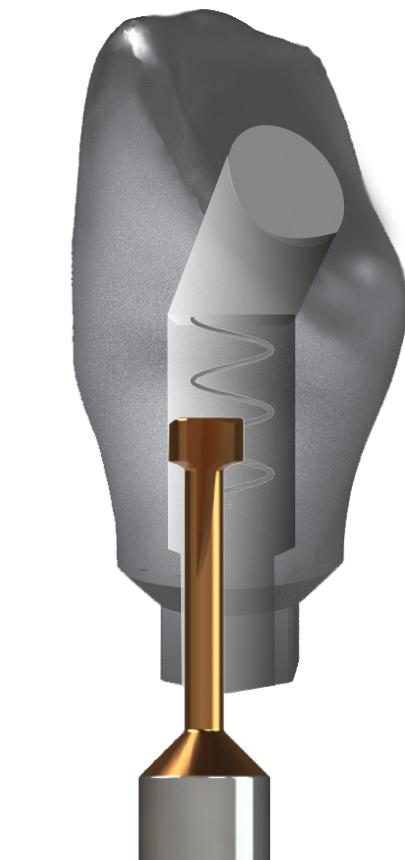


CAD

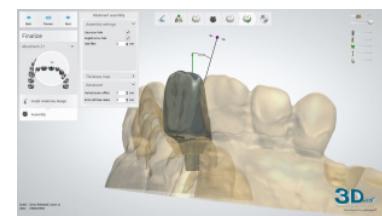

3shape ▶




exocad

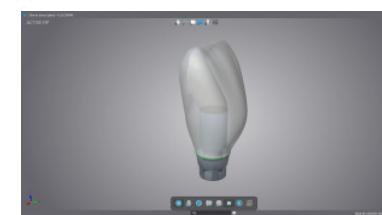


dental wings


CAM

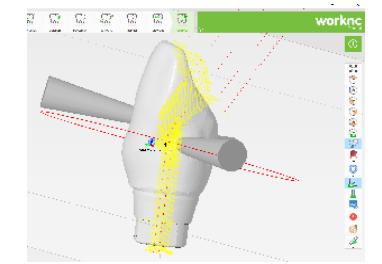

worknc
Dental

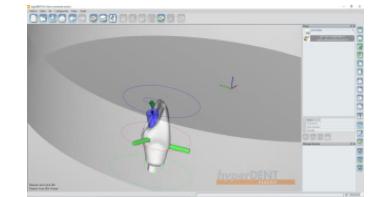

→ FOLLOW-ME I
TECHNOLOGY GROUP

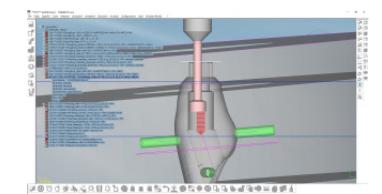

MILL
BOX | sum3D


DIGITAL ANALOG




CAD-CAM



3shape ▶
Model Builder

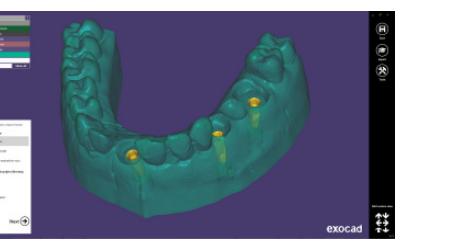

exocad
Model Creator

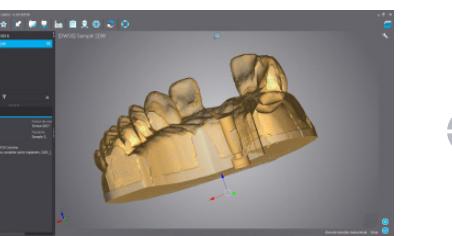

dental wings
Model Builder

DYNAMIC PRE-MILL 3D®




CAD



exocad




3shape ▶




dental wings

CAM

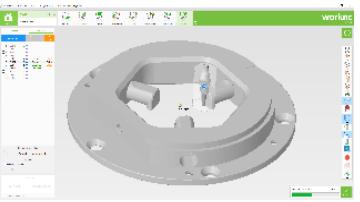

worknc
Dental

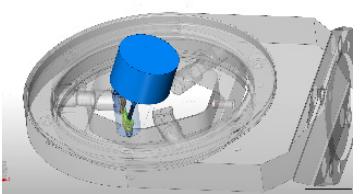

MILL
BOX | sum 3D

FOLLOW-ME I
TECHNOLOGY GROUP

*Soon

DYNAMIC SYSTEM



List of compatibilities available

AB	DSP BIOMEDICAL	NEODENT
ACE	EASY IMPLANT	NEOSS
ADIN	ECKERMANN	NOBEL BIOCARE
ALPHABIO	ELITE MEDICA	NORIS MEDICAL
ANCLADEN	EUROTEKNIKA	NORMON
ANKYLOS	GALIMPLANT	NOVA IMPLANTS
ANTHOGYR	GC TECH	OSSTEM IMPLANT
ARDS	GLOBAL D (TEKKA)	OSTEOPLUS
ASTRA	GMI (ILERIMPLANT)	PALTOP
AVINENT	GT MEDICAL	PHIBO
BEGO	HAHN IMPLANT (GLIDEWELL)	PROCLINIC
BIOCONCEPT	HI-TEC	RADHEX
BIOGENESIS	HIOSEN	SEWON MEDIX
BIOHORIZONS	IBS	SGS
BIOMET 3i	IDO IMPLANTS	SIC INVENT
BIOLOK	IHDE DENTAL (IMBIODENT)	SIGNO VINCES
BIONER	IMPLANT DIRECT	SOUTHERN IMPLANTS
BIOTEC	IMPLANT GENESIS	STERNGOLD
BIOTECH	INTRA-LOCK	STRAUMANN
BREDENT MEDICAL	JDENTALCARE	SYBRON IMPLANT SOLUTIONS
BTI	KEYSTONE	TITANIUM - FIX
BTK	KLOCKNER	TRE-OSS
B&W	LASAK	TRI DENTAL IMPLANTS
CAMLOG	LEADER	TRINON
CONEXÃO SISTEMA DE PRÓTESE	MEDENTIS	UFIT
CORTEX	MEGAGEN	VULKAN IMPLANTS
DENTAL TECH	MICRODENT	XIVE
DENTAURUM	MIS	YES IMPLANT
DENTIS	MOZO-GRAU	ZACOM (OSSEOLIFE)
DENTIUM	MPI	ZIMMER
DIO IMPLANTS	NEOBIOTECH	

AB

- ✿ I2
Implant: Ø 3,5/3,75/4,2/4,5/ 5/6
Platform: Standard (Code 0040) p. 87
- ✿ I22
Implant: Ø 3,75/4,22
Platform: Standard (Code 0040) p. 87
- ✿ I5
Implant: Ø 3,5/3,75/4,2/4,5/5/6/7/8
Platform: Standard (Code 0040) p. 87
- ✿ I55
Implant: Ø 3,75/4,2/4,5/5/6/7/8
Platform: Standard (Code 0040) p. 87
- ✿ I10
Implant: Ø 4,2/5
Platform: Standard (Code 0040) p. 87
- ✿ I15
Implant: Ø 6/7/8
Platform: Standard (Code 0040) p. 87
- ✿ Multi Unit D1-P64
Platform: Universal (Code 0025) p. 76

ACE

- ✿ External Hex
Implant: Ø 3,3
Platform: NP 3,5 (Code 0023) p. 74
- Implant: Ø 3,75/4
Platform: RP 4,1 (Code 0024) p. 75
- Implant: Ø 4,75
Platform: WP 5 (Code 0058) p. 102

- ✿ Infinity TRI-CAM
Implant: Ø 3,5
Platform: 3,5 (Code 0026) p. 77
- Implant: Ø 4,3
Platform: 4,3 (Code 0027) p. 78
- Implant: Ø 5
Platform: 5 (Code 0028) p. 79
- ✿ Infinity Internal Hex
Implant: Ø 3,7/4,1
Platform: 3,5 (Code 0040) p. 87
- Implant: Ø 4,7/5,1
Platform: 4,5 (Code 0041) p. 89
- ✿ Infinity Octagon
Implant: Ø 3,3/4,1/4,8
Platform: RP 4,8 (Code 0037) p. 84
- Implant: Ø 4,8
Platform: WP 6,5 (Code 0096) p. 119
- ✿ Multi Unit
Platform: Universal (Code 0025) p. 76

ADIN

- ✿ Swell
Implant: Ø 3,3
Platform: 3,45 (Code 0040) p. 87
- Implant: Ø 3,75/4,2
Platform: 3,6 (Code 0040) p. 87
- Implant: Ø 5
Platform: 4 (Code 0040) p. 87
- Implant: Ø 6
Platform: 4,6 (Code 0040) p. 87

- ✿ Touareg-S / Touareg-OS
Implant: Ø 3,5
Platform: 3,45 (Code 0040) p. 87
- Implant: Ø 4,3
Platform: 3,6 (Code 0040) p. 87
- Implant: Ø 5
Platform: 4 (Code 0040) p. 87
- Implant: Ø 6
Platform: 5 (Code 0040) p. 87
- ✿ Touareg CloseFit
Implant: Ø 3,5
Platform: RP (Code 0021) p. 72
- Implant: Ø 4,3/5
Platform: WP (Code 0022) p. 73
- ✿ Multi Unit TMA
Platform: Universal (Code 0025) p. 76

ALPHABIO

- ✿ Internal Hex Connection (IH) SPI
Implant: Ø 3,3/3,75/4,2/5/6
Platform: Universal (Code 0040) p. 87
- ✿ Internal Hex Connection (IH) ICE
Implant: Ø 3,7/3,75/4,2/4,65/5,3
Platform: Universal (Code 0040) p. 87
- ✿ Internal Hex Connection (IH) DFI
Implant: Ø 3,3/3,75/4,2/4,5
Platform: Universal (Code 0040) p. 87
- ✿ Internal Hex Connection (IH) ATID
Implant: Ø 3,3/3,75/4,2/5/6
Platform: Universal (Code 0040) p. 87
- ✿ Internal Hex Connection (IH) NEO
Implant: Ø 3,75/4,2/5
Platform: 3,5 (Code 0040) p. 87

- ✿ Conical Hex Connection (CHC) NICE
Implant: Ø 3,2
Platform: Narrow (Code 0136) p. 135
 - ✿ Conical Hex Connection (CHC) NEO
Implant: Ø 3,2/3,5
Platform: Narrow (Code 0136) p. 135
 - ✿ Conical Standard Connection (CS)
Implant: Ø 3,75/4,2/5
Platform: Standard (Code 0169) p. 151
- ANCLADEN**
- ✿ Anclalock
Implant: Ø 3,75/4,25/5
Platform: 3,5 (Code 0040) p. 87
- ANKYLOS**
- ✿ Ankylos
Implant: Ø 3,5
Platform: 3,5 (Code 0075) p. 108
 - Implant: Ø 4,5
Platform: 4,5 (Code 0075) p. 108
 - Implant: Ø 5,5
Platform: 5,5 (Code 0075) p. 108
 - Implant: Ø 7
Platform: 7 (Code 0075) p. 108
- ANTHOGYR**
- ✿ Axiom REG / PX
Implant: Ø 3,4
Platform: 3,4 (Code 0161) p. 143
 - Implant: Ø 4
Platform: 4 (Code 0149) p. 137
 - Implant: Ø 4,6
Platform: 4,6 (Code 0149) p. 137
 - Implant: Ø 5,2
Platform: 5,2 (Code 0162) p. 144

- ✿ Anthofit HE
Implant: Ø 3,5/3,75/4
Platform: R (4,1) (Code 0024) p. 75
 - Implant: Ø 5
Platform: L (5) (Code 0058) p. 102
 - ✿ Ossfit
Implant: Ø 3,5/4,2
Platform: 4,8 (Code 0074) p. 107
 - Implant: Ø 3,5/4,2
Platform: 4,8 (Code 0037) p. 84
 - Implant: Ø 5
Platform: 6,5 (Code 0096) p. 119
 - ✿ Multi Unit
Implant: Ø 4,8
Platform: Universal (Code 0163) p. 145
- ARDS**
- ✿ Smart
Implant: Ø 3,75/4,2/4,5
Platform: 3,75 (Code 0040) p. 87
 - ✿ Classic
Implant: Ø 3,75/4,2/4,5
Platform: 3,75 (Code 0040) p. 87
 - Implant: Ø 3,3/3,75/4,2/5/6
Platform: 3,75 (Code 0040) p. 87
 - ✿ Premium
Implant: Ø 3,3/3,75/4,2/5/6
Platform: 3,75 (Code 0040) p. 87
 - ✿ CIT
Implant: Ø 3,3/3,75/4,2/5/6
Platform: 3,75 (Code 0040) p. 87

- ASTRA**
- ✿ Yellow
Implant: Ø 3
Platform: Yellow (Code 0109) p. 122
 - ✿ Aqua
Implant: Ø 3,5/4
Platform: Aqua (Code 0004) p. 55
 - ✿ Lilac
Implant: Ø 4,5/5
Platform: Lilac (Code 0005) p. 56
 - ✿ Cono 20°
Platform: Regular/Wide (Code 0066) p. 106
 - ✿ Evolution (Internal)
Implant: Ø 3
Platform: 3,0 (Code 0090) p. 116
 - Implant: Ø 3,6
Platform: 3,6 (Code 0006) p. 57
 - Implant: Ø 4,2
Platform: 4,2 (Code 0007) p. 58
 - Implant: Ø 4,8
Platform: 4,8 (Code 0091) p. 117
 - Implant: Ø 5,4
Platform: 5,4 (Code 0092) p. 118
 - ✿ Uni Abutment
Platform: Universal (Code 0008) p. 59

AVINENT

- ★ HE/EC
 - Implant: Ø 3,3/3,8/4/4,2/4,8//4,5/5
 - Platform: 4,1 (Code 0024) p. 75
 - Implant: Ø 4,8
 - Platform: 5,1 (Code 0061) p. 105
- ★ HI/IC
 - Implant: Ø 3,1//3,5/4
 - Platform: 3,5 (Code 0040) p. 87
 - Implant: Ø 3,3/3,8/4/4,2/4,8//4,5/5
 - Platform: 4,1 (Code 0040) p. 87
- ★ Transepitelial
 - Platform: Regular (Code 0025) p. 76

BEGO

- ★ RS/RSX
 - Implant: Ø 3,0
 - Platform: 3,0 (Code 0049) p. 96
- ★ S/RI/RS/RSX
 - Implant: Ø 3,25/3,75
 - Platform: 3,67 (Code 0050) p. 97
 - Implant: Ø 4,1
 - Platform: 4,1 (Code 0051) p. 98
 - Implant: Ø 4,5
 - Platform: 4,5 (Code 0052) p. 99
 - Implant: Ø 5,5
 - Platform: 5,5 (Code 0081) p. 110
- ★ MINI
 - Implant: Ø 2,7/2,9/3,1
 - Platform: Mini (Code 0187) p. 157
- ★ MULTIPLUS
 - Platform: Universal (Code 0150) p. 138

BIOCONCEPT

- ★ BC Tissue Level Standard
 - Implant: Ø 3,3/4,1/4,8
 - Platform: Regular (Code 0037) p. 84
- ★ BC Tissue Level Standard Plus
 - Implant: Ø 4,8
 - Platform: Regular (Code 0037) p. 84
- ★ BC Tissue Level Tapered Effect
 - Implant: Ø 4,8
 - Platform: Regular (Code 0037) p. 84
- ★ BC Bone Level
 - Implant: Ø 3,3
 - Platform: Narrow (Code 0033) p. 82
 - Implant: Ø 4,1/4,8
 - Platform: Regular (Code 0035) p. 83
- ★ BV Tapered Bone Level
 - Implant: Ø 3,5
 - Platform: Narrow (Code 0029) p. 80
 - Implant: Ø 4/4,5/5
 - Platform: Regular (Code 0030) p. 81
- ★ BIOGENESIS
 - ★ 3icon
 - Implant: Ø 3,3
 - Platform: Mini (Pink) (Code 0023) p. 74
 - Implant: Ø 3,75/4/4,3/4,5
 - Platform: Regular (Blue) (Code 0024) p. 75
 - Implant: Ø 5/5,5
 - Platform: Wide (Yellow) (Code 0058) p. 102
 - ★ Aticon
 - Implant: Ø 3,5/4/4,5/5
 - Platform: Blue (Code 0005) p. 56
 - ★ Aticon (Cone 20°)
 - Platform: Regular/Wide (Code 0066) p. 106

Iticon

- ★ BC Tissue Level Standard
 - Implant: Ø 3,3/4,1/4,8
 - Platform: 4,8 (Code 0037) p. 84

BIOHORIZONS

- ★ Tapered Internal
 - Implant: Ø 3/3,4
 - Platform: 3 (Grey) (Code 0102) p. 121
- ★ BC Tissue Level Tapered Effect
 - Implant: Ø 3,8
 - Platform: 3,5 (Yellow) (Code 0040) p. 87
- ★ BC Bone Level
 - Implant: Ø 4,6
 - Platform: 4,5 (Green) (Code 0041) p. 89
- ★ Internal
 - Implant: Ø 3,5/4
 - Platform: 3,5 (Yellow) (Code 0040) p. 87
 - Implant: Ø 4/5
 - Platform: 4,5 (Green) (Code 0041) p. 89
 - Implant: Ø 5/6
 - Platform: 5,7 (Blue) (Code 0080) p. 109

BIOMET 3i

- ★ Osseotite
 - Implant: Ø 3,25
 - Platform: 3,4 (Code 0003) p. 54
- Implant: Ø 3,75/4
 - Platform: 4,1 (Code 0024) p. 75
- Implant: Ø 5
 - Platform: 5 (Code 0058) p. 102

Certain

- ★ Certain
 - Implant: Ø 3,25/4
 - Platform: 3,4 (Code 0001) p. 52

Low Profile

- ★ Low Profile
 - Platform: Universal (Code 0025) p. 76

BIOLOK

- ★ External Hexagon
 - Implant: Ø 3,45
 - Platform: 3,45 (Code 0003) p. 54

BIONER

- ★ Ikelt / Bikelt
 - Implant: Ø 3,3/3,75/4
 - Platform: 4,1 (Code 0024) p. 75

Ikelt

- ★ Ikelt
 - Implant: Ø 5
 - Platform: 5 (Code 0058) p. 102

Hikelt

- ★ Hikelt
 - Implant: Ø 3,8
 - Platform: 3,95 (Code 0040) p. 87
 - Implant: Ø 4,7
 - Platform: 4,9 (Code 0041) p. 89

TopDM

- ★ TopDM
 - Implant: Ø 3,5
 - Platform: 3,5 (Code 0021) p. 72
 - Implant: Ø 4
 - Platform: 4 (Code 0021) p. 72
 - Implant: Ø 5
 - Platform: 5 (Code 0021) p. 72

Transepitelial A-5M

- ★ Transepitelial A-5M
 - Platform: Regular (Code 0025) p. 76

BIOTEC

- ★ SPR/CIM
 - Implant: Ø 3,3
 - Platform: 3,3 (Code 0040) p. 87

SPR/SPTT/CIM

- ★ SPR/SPTT/CIM
 - Implant: Ø 4,2
 - Platform: 4,2 (Code 0040) p. 87
 - Implant: Ø 5
 - Platform: 5 (Code 0040) p. 87

BIOTECH

- ★ Kontakt
 - Implant: Ø 3
 - Platform: Yellow Narrow (Code 0164) p. 146
- Implant: Ø 3,6/4,2/4,8/5,4
 - Platform: Regular (Code 0165) p. 147

BREDENT MEDICAL

- ★ Narrow Sky
 - Implant: Ø 3,5
 - Platform: NP 3,5 (Code 0110) p. 123
- ★ Blue Sky
 - Implant: Ø 3,5/4/4,5/5,5
 - Platform: 4 (Code 0111) p. 124
- ★ Blue Sky Classic
 - Implant: Ø 3,5/4/4,5
 - Platform: 4 (Code 0111) p. 124

BTI

- ★ External Connection Tiny
 - Implant: Ø 2,5/3/3,3/3,5/3,75
 - Platform: Tiny 3,5 (Code 0009) p. 60

External Connection

- ★ External Connection
 - Implant: Ø 3,75/4/4,5/5
 - Platform: Universal 4,1 (Code 0024) p. 75
 - Implant: Ø 4,5/5,5
 - Platform: Ancha 5,5 (Code 0060) p. 104

Internal Connection

- ★ Internal Connection
 - Implant: Ø 3,3/3,5/3,75/4/4,25/4,5/5/5,5
 - Platform: Universal 4,1 (Code 0010) p. 61
 - Implant: Ø 5/5,5/6,25
 - Platform: Ancha 5,5 (Code 0059) p. 103

Multi-IM

- ★ Multi-IM
 - Platform Universal 4,1 (Code 0151) p. 139

BTK

- ★ Klassic / Konic
 - Implant: Ø 3,25
 - Platform: 3,4 EN (Code 0003) p. 54
 - Implant: Ø 3,25PL/3,75/4
 - Platform: 4,1 ER (Code 0024) p. 75
 - Implant: Ø 3,25/4
 - Platform: 3,5 IR (Code 0040) p. 87

B&W

- ★ External Hexagon
 - Implant: Ø 3,75/4
 - Platform: 4,1 (Code 0024) p. 75
 - Implant: Ø 5
 - Platform: 5 (Code 0058) p. 102

Internal Hexagon

- ★ Internal Hexagon
 - Implant: Ø 3,3/4
 - Platform: 4 (Code 0040) p. 87

CAMLOG

★ Camlog Screw-Line

Implant: Ø 3,8
Platform: 3,8 (Code 0011) p. 62

Implant: Ø 4,3
Platform: 4,3 (Code 0012) p. 63

★ Conelog Screw-Line

Implant: Ø 3,8
Platform: 3,8 (Code 0120) p. 125

Implant: Ø 4,3
Platform: 4,3 (Code 0121) p. 126

CONEXÃO SISTEMA DE PRÓTESE

★ Flash

Implant: Ø 3,5/4,3/5
Platform: Universal (Code 0021) p. 72

★ Torq

Implant: Ø 3,5/3,75/4
Platform: Universal (Code 0021) p. 72

★ Expand

Implant: Ø 3,75/4/5
Platform: Universal (Code 0021) p. 72

CORTEX

★ Dynamix

Implant: Ø 3,3/3,8/4,2/5/6
Platform: 3,75 (Code 0040) p. 87

★ Classix

Implant: Ø 3,3/3,8/4,2/5/6
Platform: 3,75 (Code 0040) p. 87

★ Saturn

Implant: Ø 3,8/4,2
Platform: 3,5 (Code 0040) p. 87

★ Conical Platform:

Implant: Ø 3
Platform: NP (Code 0109) p. 122

Implant: Ø 3,3/3,8/4,2
Platform: RP (Code 0004) p. 55

Implant: Ø 5/6
Platform: WP (Code 0005) p. 56

★ Magix

Implant: Ø 3,3/3,8/4,2
Platform: RP (Code 0004) p. 55

★ Multi Unit

Platform Universal (Code 0025) p. 76

DENTAL TECH

★ Implogic

Implant: Ø 4,5
Platform: 4,5 (Blue) (Code 0041) p. 89

DENTAURUM

★ Tiologic

Implant: Ø 3,3
Platform: Small (Code 0130) p. 131

Implant: Ø 3,7/4,2
Platform: Medium (Code 0131) p. 132

Implant: Ø 4,8/5,5
Platform: Large (Code 0132) p. 133

DENTIS

★ s-Clean

Implant: Ø 3,7
Platform: Mini (Code 0030) p. 81

Implant: Ø 4,1/4,3
Platform: Regular (Code 0030) p. 81

Implant: Ø 4,8
Platform: Wide (Code 0030) p. 81

DENTIUM

★ SimpleLine II

Implant: Ø 3,8/4,3
Platform: 4,8 (Code 0074) p. 107

Implant: Ø 3,8/4,3
Platform: 4,8 (Code 0037) p. 84

Implant: Ø 4,3/4,8
Platform: 6,5 (Code 0096) p. 119

★ SuperLine and Implantium

Implant: Ø 3,4
Platform: 3,6 (Code 0030) p. 81

Implant: Ø 3,8
Platform: 4 (Code 0030) p. 81

Implant: Ø 4,3
Platform: 4,5 (Code 0030) p. 81

Implant: Ø 4,8
Platform: 5 (Code 0030) p. 81

Implant: Ø 4,8
Platform: 6 (Code 0030) p. 81

DIO IMPLANTS

★ SM System

Implant: Ø 4,5/5/5,3
Platform: Regular/Wide (Code 0013) p. 64

★ UF II Narrow

Implant: Ø 3/3,3
Platform: Narrow (Code 0014) p. 65

★ UF II

Implant: Ø 3,8/4/4,5/5/5,5
Platform: Regular (Code 0030) p. 81

★ External

Implant: Ø 3,3/3,8
Platform: Narrow 3,5 (Code 0023) p. 74

Implant: Ø 3,75/4/4,5
Platform: Regular 4,1 (Code 0024) p. 75

Implant: Ø 5/5,3/5,5/6
Platform: Wide 5,1 (Code 0061) p. 105

DSP BIOMEDICAL

★ External Hexagon

Implant: Ø 3,75/4/5//3,5/3,8/4,3
Platform: 4,1 (Code 0024) p. 75

EASY IMPLANT

★ Master C

Implant: Ø 3,5
Platform: 3,5 (Ocean) (Code 0004) p. 55

Implant: Ø 4
Platform: 4 (Ocean) (Code 0004) p. 55

Implant: Ø 4,5
Platform: 4,5 (Lilas) (Code 0030) p. 81

Implant: Ø 5
Platform: 5 (Lilas) (Code 0030) p. 81

★ Master S

Implant: Ø 3,3
Platform: 3,3 (Ocean) (Code 0004) p. 55

Implant: Ø 3,75
Platform: 3,75 (Lilas) (Code 0030) p. 81

Implant: Ø 4,25
Platform: 4,25 (Lilas) (Code 0030) p. 81

Implant: Ø 4,75
Platform: 4,75 (Lilas) (Code 0030) p. 81

★ Master L

Implant: Ø 3,3
Platform: 3,3 (Lilas) (Code 0030) p. 81

Implant: Ø 3,75
Platform: 3,75 (Lilas) (Code 0030) p. 81

Implant: Ø 4,25
Platform: 4,25 (Lilas) (Code 0030) p. 81

Implant: Ø 4,75
Platform: 4,75 (Lilas) (Code 0030) p. 81

★ Multi Unit Conical Abutment

Platform Universal (Code 0025) p. 76

ECKERMANN

★ Hexagon

Implant: Ø 3,3/4/4,5/5
Platform: 4,1 (Code 0024) p. 75

ELITE MEDICA

★ External Connection

Implant: Ø 3,75
Platform: Narrow (Code 0023) p. 74

Implant: Ø 4
Platform: 4 (Ocean) (Code 0004) p. 55

Implant: Ø 4,5
Platform: 4,5 (Lilas) (Code 0030) p. 81

Implant: Ø 5
Platform: Wide (Code 0061) p. 107

EUROTEKNIKA

★ Naturactis

Implant: Ø 3,5
Platform: 3,4 (Code 0004) p. 55

Implant: Ø 4,5
Platform: 3,75 (Lilas) (Code 0030) p. 81

Implant: Ø 4,25
Platform: 4,25 (Lilas) (Code 0030) p. 81

Implant: Ø 4,75
Platform: 4,75 (Lilas) (Code 0030) p. 81

★ Uneva

Implant: Ø 3,6
Platform: 4,1 (Code 0024) p. 75

Implant: Ø 4,1
Platform: 4,1 (Code 0024) p. 75

★ Uneva (Platform: Switching)

Implant: Ø 4,8
Platform: 4,1 (Code 0024) p. 75

Implant: Ø 6
Platform: 4,1 (Code 0024) p. 75

Natea

Implant: Ø 3,6/4,1/4,8
Platform: Narrow (Code 0004) p. 55

Implant: Ø 3,6/4,1/4,8
Platform: Regular (Code 0004) p. 55

Implant: Ø 6
Platform: Wide (Code 0004) p. 55

Aesthetica

Implant: Ø 4,1
Platform: 4,8 (Code 0074) p. 107

Implant: Ø 4,1
Platform: 4,8 (Code 0037) p. 84

Implant: Ø 4,8
Platform: 6,5 (Code 0096) p. 119

Naturall

Implant: Ø 3,5
Platform: Narrow (Code 0004) p. 55

Implant: Ø 4,5
Platform: Regular (Code 0004) p. 55

Implant: Ø 5
Platform: Wide (Code 0004) p. 55

★ Multi Unit Tetra

Platform Universal (Code 0025) p. 76

GALIMPLANT

★ External Connection

Implant: Ø 3,5/4
Platform: 4 (Code 0024) p. 75

★ Internal Connection

Implant: Ø 3,5
Platform: 3,5 (Code 0004) p. 55

Implant: Ø 4
Platform: 4 (Code 0004) p. 55

Implant: Ø 5
Platform: 5 (Code 0004) p. 55

★ AbutmentMulti-Position

Platform: Universal (Code 0025) p. 76

GC TECH

★ AADVA Standard / Tapered Implants

Implant: Ø 3,3
Platform: Narrow (Code 0196) p. 158

Implant: Ø 4
Platform: Regular (Code 0197) p. 159

Implant: Ø 5
Platform: Wide (Code 0198) p. 160

GLOBAL D (TEKKA)

★ In-Kone Universal

Implant: Ø 3,5/4/4,5/5
Platform: 5 (Code 0152) p. 140

★ In-Kone Primo

Implant: Ø 3,5/4/4,5/5
Platform: 5 (Code 0152) p. 140

GMI (ILERIMPLANT)

★ Phoenix

Implant: Ø 3,3/3,75/4
Platform: Standard 4,1 (Code 0024) p. 75

Implant: Ø 5
Platform: Wide 5,1 (Code 0061) p. 105

★ Frontier

Implant: Ø 3,3/3,75/4,25
Platform: RP 3,3 (Code 0040b) p. 88

Implant: Ø 4,75/5,75
Platform: WP 4,3 (Code 0041b) p. 90

★ Universal

Platform: PS-RP 4,8 (Code 0025) p. 76

GT MEDICAL

★ Best Fit Internal Octagon

Implant: Ø 3,7/4,3/4,8
Platform: Regular (Code 0074) p. 107

Implant: Ø 3,7/4,3/4,8
Platform: Regular (Code 0037) p. 84

★ Best Fit Internal Hexagon

Implant: Ø 3,7/4,1/4,3/4,8
Platform: Wide (Code 0005) p. 56

★ Best Fit External Hexagon

Implant: Ø 3,5
Platform: Narrow (Code 0023) p. 74

Implant: Ø 4,1
Platform: Regular (Code 0024) p. 75

Implant: Ø 5,1
Platform: Wide (Code 0061) p. 105

HAHN IMPLANT (GLIDEWELL)

★ Hahn Tapered Implant

Implant: Ø 3,5/4,3
Platform: Standard 4,1 (Code 0021) p. 72

Implant: Ø 5
Platform: 5 (Code 0022) p. 73

Implant: Ø 7
Platform: 7 (Code 0124) p. 127

★ Multi Unit Abutment system

Platform: Universal (Code 0025) p. 76

HI-TEC

★ Tapered Self Thread

Implant: Ø 3,3/3,75
Platform: 3,5 (Code 0040) p. 87

Implant: Ø 4,2/5
Platform: 4,5 (Code 0041) p. 89

★ Logic Plus

Implant: Ø 3,5
Platform: 3,7 (Code 0040) p. 87

Implant: Ø 4,3
Platform: 3,9 (Code 0040) p. 87

HIOSEN

★ ETI SA/ETIII SA

Implant: Ø 3,5
Platform: Mini (Code 0029) p. 80

Implant: Ø 4/4,5/5
Platform: Regular (Code 0030) p. 81

★ ETI BA

Implant: Ø 3,5
Platform: Mini (Code 0029) p. 80

Implant: Ø 4/4,5/5
Platform: Regular (Code 0030) p. 81

IBS

★ Magic FC

Implant: Ø 4/4,5/5,5/6/6,5
Platform: 3,8 (Code 0030) p. 81

★ N.R Fix

Implant: Ø 3/3,5
Platform: 3,8 (Code 0030) p. 81

IDO IMPLANTS

★ IDo Implant

Implant: Ø 3,8/4,4,5/5,5/6/7
Platform: Universal (Code 0030) p. 81

IHDE DENTAL (IMBIODENT)

★ Bone Level Plus

Implant: Ø 3,3
Platform: 3,3 (Code 0033) p. 82

Implant: Ø 4,1
Platform: 4,1 (Code 0035) p. 83

Implant: Ø 4,8
Platform: 4,8 (Code 0035) p. 83

IMPLANT DIRECT

★ RePlus / Replant / Reactive

Implant: Ø 3,5/3,7/4,2
Platform: 3,5 (Code 0026) p. 77

Implant: Ø 4,3/4,7
Platform: 4,3 (Code 0027) p. 78

Implant: Ø 5/5,7
Platform: 5 (Code 0028) p. 79

★ Legacy

Implant: Ø 3,7/4,2
Platform: 3,5 (Code 0040) p. 87

Implant: Ø 4,7/5,2
Platform: 4,5 (Code 0041) p. 89

★ Swishplant / Swishplus

Implant: Ø 4,1/4,8
Platform: 4,8 (Code 0074) p. 107

Implant: Ø 4,1/4,8
Platform: 4,8 (Code 0037) p. 84

Implant: Ø 4,8/5,7
Platform: 6,5 (Code 0096) p. 119

★ SwishActive

Implant: Ø 3,3
Platform: 3 (Code 0021) p. 72

Implant: Ø 4,1/4,8
Platform: 3,4 (Code 0022) p. 73

★ Interactive

Implant: Ø 3,2/3,7
Platform: 3 (Code 0021) p. 72

Implant: Ø 4,3/5
Platform: 3,4 (Code 0022) p. 73

IMPLANT GENESIS

★ Aktiv System

Implant: Ø 3,5/3,75/4,2/5
Platform: Standard (Code 0040) p. 87

INTRA-LOCK

★ Unihex

Implant: Ø 4
Platform: Regular (Code 0024) p. 75

Implant: Ø 4,75
Platform: Wide (Code 0024) p. 75

★ IntraHex

Implant: Ø 3,75/4
Platform: 3,5 (Code 0040) p. 87

Implant: Ø 4,75
Platform: 4,5 (Code 0041) p. 89

JDENTALCARE

★ JDEvolution/JDEvolution Plus

Implant: Ø 3,7
Platform: 3,7 (Code 0040) p. 87

Implant: Ø 4,3/5
Platform: 4 (Code 0040) p. 87

Implant: Ø 6
Platform: 5 (Code 0040) p. 87

★ JD ICON

Implant: Ø 3,9
Platform: 3,9 (Code 0022) p. 73

Implant: Ø 4,3
Platform: 4 (Code 0022) p. 73

Implant: Ø 5
Platform: 4,7 (Code 0022) p. 73

KEYSTONE

★ Internal TiLobe PrimaConnex

Implant: Ø 3,3/3,5
Platform: 3,5 (Code 0044) p. 91

Implant: Ø 4/4,1
Platform: 4,1 (Code 0045) p. 92

Implant: Ø 5
Platform: 5 (Code 0046) p. 93

★ Restore

Implant: Ø 3,75/4
Platform: RD 4,1 (Code 0024) p. 75

KLOCKNER

- ◆ Essential Cone
 - Implant: Ø 3,5/4/4,5
Platform: 4,5 (Code 0054) p. 100

KL

- ◆ KL
 - Implant: Ø 3,5
Platform: Narrow (Code 0023) p. 74
 - Implant: Ø 4,1
Platform: Regular (Code 0024) p. 75
 - Implant: Ø 5,1
Platform: Wide (Code 0061) p. 105

Vega

- ◆ Vega
 - Implant: Ø 3,5
Platform: NV (Code 0082) p. 111
 - Implant: Ø 4/4,5
Platform: RV (Code 0083) p. 112

LASAK

- ◆ Bioniq
 - Implant: Ø 2,9
Platform: QN (Yellow) (Code 0166) p. 148
 - Implant: Ø 3,5/4/5
Platform: QR (Blue) (Code 0167) p. 149

Multi Unit

- ◆ Multi Unit
 - Implant: Ø
Platform: Universal (Code 0168) p. 150

LEADER

- ◆ Tixos Internal Hex
 - Implant: Ø 3,3
Platform: 3,5 (Code 0040) p. 87
 - Implant: Ø 3,75
Platform: 4 (Code 0040) p. 87
- ◆ Tixos External Hex
 - Implant: Ø 3,3/3,75
Platform: 4,1 (Code 0024) p. 75

Tixos External Hex

- Implant: Ø 5
Platform: 5 (Code 0058) p. 102

MEDENTIS

- ◆ ICX-Templant
 - Implant: Ø 3,75
Platform: 3,75 (Code 0125) p. 128
 - Implant: Ø 4,1
Platform: 4,1 (Code 0125) p. 128
 - Implant: Ø 4,8
Platform: 4,8 (Code 0125) p. 128

MEGAGEN

- ◆ AnyRidge
 - Implant: Ø 3,5
Platform: Small (Code 0015) p. 66
 - Implant: Ø 4/4,5
Platform: Regular (Code 0015) p. 66
 - Implant: Ø 5/5,5
Platform: Wide (Code 0015) p. 66

AnyOne Internal

- ◆ AnyOne Internal
 - Implant: Ø 3,5/4/4,5/5/6/7
Platform: General (Code 0030) p. 81

AnyOne External

- ◆ AnyOne External
 - Implant: Ø 3,5
Platform: Small 3,5 (Code 0023) p. 74

- Implant: Ø 4
Platform: Regular 4,1 (Code 0024) p. 75

- Implant: Ø 4,5
Platform: Regular 4,5 (Code 0024) p. 75

- Implant: Ø 5
Platform: Wide 5 (Code 0058) p. 102

- Implant: Ø 6
Platform: SuperWide 5,5 (Code 0058) p. 102

Cone Abutment

- Implant: Ø Universal
Platform: 3,8 (Code 0128) p. 129
- Implant: Ø Universal
Platform: 4,8 (Code 0074) p. 107

MINI NARROW RIDGE

- ◆ Mini Narrow Ridge
 - Implant: Ø 3/3,4
Platform: Mini (Code 0014) p. 65

Multi Unit N Type

- ◆ Multi Unit N Type
 - Platform: Universal (Code 0025) p. 76

MICRODENT

- ◆ Universal
 - Implant: Ø 2,8/3,25
Platform: 3,5 (Code 0003) p. 54
 - Implant: Ø 3,3/3,5/3,75/4
Platform: 4,1 (Code 0024) p. 75
 - Implant: Ø 4,2/5
Platform: 5,1 (Code 0058) p. 102

System

- ◆ System
 - Implant: Ø 2,8/3,25
Platform: 3,5 (Code 0003) p. 54

Ektos

- ◆ Ektos
 - Implant: Ø 3,7/4,2
Platform: 3,5 (Code 0040b) p. 88

MIS

- ◆ Lance
 - Implant: Ø 3,75/4,2
Platform: Standard (Code 0024) p. 75

- Implant: Ø 4,5
Platform: Wide (Code 0058) p. 102

- Implant: Ø 5
Platform: Wide 5 (Code 0058) p. 102

- Implant: Ø 6
Platform: General (Code 0020) p. 71

Seven

- Implant: Ø 3,3
Platform: Narrow (Code 0019) p. 70
- Implant: Ø 3,75/4,2
Platform: Standard (Code 0040) p. 87
- Implant: Ø 5/6
Platform: Wide (Code 0041) p. 89

M4

- ◆ M4
 - Implant: Ø 3,3
Platform: Narrow (Code 0019) p. 70

- ◆ Multi Unit N Type
 - Implant: Ø 3,75/4,2
Platform: Standard (Code 0040) p. 87

- ◆ C1
 - Implant: Ø 5/6
Platform: Wide (Code 0041) p. 89

C1

- ◆ C1
 - Implant: Ø 3,3
Platform: Narrow (Code 0016) p. 67

- ◆ V3
 - Implant: Ø 3,75/4,2
Platform: Standard (Code 0017) p. 68

V3

- ◆ V3
 - Implant: Ø 5
Platform: Wide (Code 0018) p. 69

MOZO-GRAU

- ◆ MG Osseous
 - Implant: Ø 3,3
Platform: 3,4 Mini (Code 0003) p. 54
 - Implant: Ø 3,4/3,75/4,25
Platform: 4,1 Standard (Code 0024) p. 75
 - Implant: Ø 5
Platform: 5 Maxi (Code 0061) p. 105

MG Inhex

- ◆ MG Inhex
 - Implant: Ø 3,3
Platform: 2,3 Mini (Code 0109) p. 122
 - Implant: Ø 3,75/4,25
Platform: 2,8 Standard (Code 0004) p. 55
 - Implant: Ø 5
Platform: 3,8 Maxi (Code 0005) p. 56

MPI

- ◆ External Connection HE Privilege
 - Implant: Ø 3,3
Platform: 3,5 (Code 0009) p. 60

- ◆ Smart HE
 - Implant: Ø 3,75/4
Platform: 4,1 (Code 0024) p. 75

- ◆ Mini Pilar CM
 - Implant: Ø 5
Platform: 5 (Code 0058) p. 102

Privilege CM

- ◆ Privilege CM
 - Implant: Ø 3,5/4
Platform: Regular (Code 0004) p. 55

- ◆ Excellence CM
 - Implant: Ø 5
Platform: Wide (Code 0005) p. 56

Excellence CM

- ◆ Excellence CM
 - Implant: Ø 3,5/4
Platform: Regular (Code 0004) p. 55
 - Implant: Ø 5
Platform: Wide (Code 0005) p. 56

NEOBIOTECH

- ◆ EB External System
 - Implant: Ø 3,5
Platform: Narrow (Code 0023) p. 74

IS Implant: System

- ◆ IS Implant: System
 - Implant: Ø 4
Platform: Regular 4 (Code 0030) p. 81
 - Implant: Ø 4,5
Platform: Regular 4,5 (Code 0030) p. 81
 - Implant: Ø 5
Platform: Wide 5 (Code 0030) p. 81
 - Platform: 4,8 (Code 0025) p. 76

NOBEL BIOCARE

- ◆ Branemark
 - Implant: Ø 3,3
Platform: Narrow (Code 0023) p. 74

- ◆ Branemark
 - Implant: Ø 3,75/4
Platform: Regular (Code 0024) p. 75

- ◆ Branemark
 - Implant: Ø 5/6
Platform: Wide (Code 0061) p. 105

Multi Unit

- ◆ Multi Unit
 - Platform: Regular (Code 0025) p. 76

NEODENT

- ◆ Helix GM/Drive GM/Titamax GM
 - Implant: Ø 3,5/3,75/4/4,3/5/6
Platform: Regular (Code 0186) p. 156

Smart HE

- ◆ Smart HE
 - Implant: Ø 3,75/4
Platform: 4,1 (Code 0024) p. 75

Mini Pilar CM

- ◆ Mini Pilar CM
 - Platform: Universal (Code 0025) p. 76

NEOSS

- ◆ ProActive Straight/Tapered
 - Implant: Ø 3,5 Green
Platform: ProActive (Code 0047) p. 94

- ◆ ProActive Straight/Tapered
 - Implant: Ø 4 Yellow
Platform: ProActive (Code 0047) p. 94

- ◆ ProActive Straight/Tapered
 - Implant: Ø 4,5 Blue
Platform: ProActive (Code 0048) p. 95

- ◆ ProActive Straight/Tapered
 - Implant: Ø 5 Peach
Platform: ProActive (Code 0048) p. 95

- ◆ ProActive Straight/Tapered
 - Implant: Ø 5,5 Lilac
Platform: ProActive (Code 0048) p. 95

NOBEL BIOCARE

- ◆ Branemark
 - Implant: Ø 3,3
Platform: Narrow (Code 0023) p. 74

- ◆ Branemark
 - Implant: Ø 3,75/4
Platform: Regular (Code 0024) p. 75

- ◆ Branemark
 - Implant: Ø 5/6
Platform: Wide (Code 0061) p. 105

Replace

- Implant: Ø 3,5
Platform: Narrow (Code 0026) p. 77
- Implant: Ø 4,3
Platform: Regular (Code 0027) p. 78
- Implant: Ø 5
Platform: Wide (Code 0028) p. 79
- Implant: Ø 6
Platform: Platform: 6 (Code 0129) p. 130

Active

- Implant: Ø 3
Platform: Mini 3.0 (Code 0159) p. 141
- Implant: Ø 3,5
Platform: Narrow (Code 0021) p. 72
- Implant: Ø 4,3/5
Platform: Regular (Code 0022) p. 73
- Implant: Ø 5,5
Platform: Wide (Code 0124) p. 127

NORIS MEDICAL

- Tuff
 - Implant: Ø 3,3/3,75/4,2/5/6
Platform: 3,75 (Code 0040) p. 87
- Tuff TT
 - Implant: Ø 3,3/3,75/4,2/5/6
Platform: 3,75 (Code 0040) p. 87
- Onix
 - Implant: Ø 3,3/3,75/4,2/5/6
Platform: 3,75 (Code 0040) p. 87
- Cortical
 - Implant: Ø 4,0/5/6
Platform: 3,75 (Code 0040) p. 87

PteryCore

- Implant: Ø 4,2
Platform: 3,75 (Code 0040) p. 87

PteryFit

- Implant: Ø 4,2
Platform: 3,75 (Code 0040) p. 87

NORMON

Normoimplant HE

- Implant: Ø 3,25/3,75/4,25/4,75
Platform: 4,1 (Code 0024) p. 75

Normoimplant HI

- Implant: Ø 3,75/4,25/4,75
Platform: 3,5 (Code 0040b) p. 88

NOVA IMPLANTS

PSI/PCI

- Implant: Ø 3,3/3,75/4,2/5/6
Platform: 3,75 (Code 0040b) p. 88

OSSTEM IMPLANT

TS

- Implant: Ø 3,5
Platform: Mini (Code 0029) p. 80

- Implant: Ø 4/4,5/5/6/7
Platform: Regular (Code 0030) p. 81

US

- Implant: Ø 3,3/3,5
Platform: Mini 3,5 (Code 0023) p. 74

- Implant: Ø 3,75/4/4,5
Platform: Regular 4,1 (Code 0024) p. 75

- Implant: Ø 5/5,5
Platform: Wide 5,1 (Code 0061) p. 105

- Implant: Ø 5/5,5
Platform: Wide PS 5 (Code 0058) p. 102

OSTEOPLUS

She

- Implant: Ø 3,45
Platform: 3,45 (Code 0009) p. 60

- Implant: Ø 3,75 / 4
Platform: 4 (Code 0024) p. 75

Shi

- Implant: Ø 3,3 / 3,75 / 4,2
Platform: 3,5 (Code 0040) p. 87

PALTOP

Advanced classic

- Implant: Ø 3,75/4,2/5
Platform: Standard (Code 0040b) p. 88

Advanced +

- Implant: Ø 3,75/4,2/5
Platform: Standard (Code 0040b) p. 88

Dynamic

- Implant: Ø 3,75/4,2/5
Platform: Standard (Code 0040b) p. 88

DIVA

- Implant: Ø 3,75/4,2/5
Platform: Standard (Code 0040b) p. 88

Conical Active

- Implant: Ø 3,75/4,2/5
Platform: Standard (Code 0029) p. 80

Universal Multi Unit

- Platform: Universal (Code 0181) p. 155

PHIBO

TSH/BNT Serie 3

- Implant: Ø 3,6
Platform: 4 (Code 0024) p. 75

TSH/BNT Serie 4

- Implant: Ø 4,2
Platform: 4 (Code 0024) p. 75

PROCLINIC

Aqua CM

- Implant: Ø 3,5/4/5
Platform: 2,82 (Code 0004) p. 55

Cylindrical External/Conical External

- Implant: Ø 3,75/4,25/3,5/4
Platform: 4,1 Estandar (Code 0024) p. 75

- Implant: Ø 5
Platform: 5 Maxi (Code 0058) p. 102

Cylindrical Internal/Conical Internal

- Implant: Ø 3,3/3,75/4,25/5//3,5/4/5
Platform: 3,5 (Code 0040) p. 87

SP Octa

- Implant: Ø 3,3/4,1/4,8
Platform: 4,8 (Code 0074) p. 107

- Implant: Ø 3,3/4,1/4,8
Platform: 4,8 (Code 0037) p. 84

- Implant: Ø 4,8
Platform: 6,5 (Code 0096) p. 119

RADHEX

PHE

- Implant: Ø 3,5
Platform: 3,5 (Code 0023) p. 74

- Implant: Ø 4/4,5/5
Platform: 4,1 (Code 0024) p. 75

PHI

- Implant: Ø 3,75
Platform: 3,5 (Code 0040b) p. 88

- Implant: Ø 4,5/5
Platform: 4,5 (Code 0041b) p. 90

SEWON MEDIX

IH2 SLA SYSTEM

- Implant: Ø 3,5
Platform: Mini (Code 0029) p. 80

- Implant: Ø 3,5/4,5/5
Platform: Regular (Code 0030) p. 81

IH2 RBM SYSTEM

- Implant: Ø 3,5
Platform: Mini (Code 0029) p. 80

- Implant: Ø 3,5/4,5/5
Platform: Regular (Code 0030) p. 81

IH SYSTEM

- Platform: Universal (Code 0025) p. 76

SGS

P1

- Implant: Ø 3,2/3,75/4,2/5/6
Platform: 3,75 (Code 0040) p. 87

P7

- Implant: Ø 3,2/3,75/4,2/4,5/5/6
Platform: 3,75 (Code 0040) p. 87

SIC INVENT

Hexagonal System SICace

- Implant: Ø 3,4/4
Platform: 3,3 (Code 0170) p. 152

- Implant: Ø 4,5/5
Platform: 4,2 (Code 0171) p. 153

SIGNO VINCES

Duo

- Implant: Ø 4,6
Platform: 4,1 (Code 0024) p. 75

Inttegra

- Implant: Ø 3,75/4
Platform: 4,1 (Code 0024) p. 75

Compact

- Implant: Ø 4,5
Platform: CM3,8 (Code 0004) p. 55

Duocon

- Implant: Ø 3,8
Platform: CM3,8 (Code 0004) p. 55

Infra

- Implant: Ø 3,3/3,8/4,6
Platform: CM (Code 0004) p. 55

SOUTHERN IMPLANTS

Tri-Nex

- Implant: Ø 3,5
Platform: 3,5 (Code 0026) p. 77

IT Connection

- Implant: Ø 3,3/4,1/4,9/5
Platform: 4,8 (Code 0037) p. 84

IT Connection

- Implant: Ø 4,9/5/6
Platform: 6,5 (Code 0096) p. 119

External Hex

Implant: Ø 3,25	
Platform: 3,4 (Code 0003)	p. 54
Implant: Ø 3,75/4	
Platform: 4,1 (Code 0024)	p. 75
Implant: Ø 4,7/5	
Platform: 5 (Code 0058)	p. 102
Implant: Ø 5,7/6	
Platform: 6 (Code 0058)	p. 102

Deep Conical

Implant: Ø 3	
Platform: 2,45 (Code 0109)	p. 122
Implant: Ø 3,5/4	
Platform: 2,95/3,1 (Code 0004)	p. 55

Internal Hex

Implant: Ø 3,75/4,2/5	
Platform: Universal (Code 0040)	p. 87

Compact Conical

Platform: 4,8 (Code 0025)	p. 76
---------------------------	-------

STERNGOLD

Implant: Ø 3,75/4/5	
Platform: 4,1 (Code 0024)	p. 75

STRAUMANN

Implant: Ø 3,3/4,1/4,8	
Platform: Regular 4,8 (Code 0037)	p. 84
Implant: Ø 4,8	
Platform: Wide 6,5 (Code 0096)	p. 119

Tissue Level NNC

Implant: Ø 3,3	
Platform: 3,5 (Code 0160)	p. 142

Synocta

Implant: Ø 4,8	
Platform: Regular 4,8 (Code 0074)	p. 107
Implant: Ø 6,5	
Platform: Wide 6,5 (Code 0137)	p. 136

Bone Level

Implant: Ø 3,3	
Platform: NC-3,3 (Code 0033)	p. 82
Implant: Ø 4,1	
Platform: RC-4,1 (Code 0035)	p. 83

Bone Level Tapered SC

Implant: Ø 2,9	
Platform: SC-2,9 (Code 0135)	p. 134

Screw-Retained

Implant: Ø Universal	
Platform: NC/RC (Code 0101)	p. 120

SYBRON IMPLANT SOLUTIONS

Endopore (Innova)

Implant: Ø 4,1	
Platform: 4,1 (Code 0024)	p. 75

TITANIUM-FIX

b-fix

Implant: Ø 3,5/4	
Platform: Regular (Code 0004)	p. 55
Implant: Ø 4,5/5	
Platform: Larga (Code 0005)	p. 56

TRE-OSS

Simple

Implant: Ø 3,3/3,75/5	
Platform: 3,75 Amarillo (Code 0040)	p. 87

TRI DENTAL IMPLANTS

TRI-Vent

Implant: Ø 3,75/4,1/4,7	
Platform: 3,5 (Code 0040)	p. 87

TRINON

Q2

Implant: Ø 3,5/3,75/4,5	
Platform: 4 (Code 0024)	p. 75

QK

Implant: Ø 4	
Platform: 4,8 (Code 0074)	p. 107
Implant: Ø 4	
Platform: 4,8 (Code 0037)	p. 84

UFIT

Gt2

Implant: Ø 3,5	
Platform: Mini (Code 0004)	p. 55
Implant: Ø 4/4,5	
Platform: Regular (Code 0005)	p. 56

Nt2

Implant: Ø 3,5	
Platform: Mini (Code 0004)	p. 55
Implant: Ø 4/4,5	
Platform: Regular (Code 0005)	p. 56

Simple

Implant: Ø 3,3/3,75/5	
Platform: 3,75 Amarillo (Code 0040)	p. 87

VULKAN IMPLANTS

IN-Hex

Implant: Ø 3,3/3,75/4,2/5	
Platform: 3,75 (Code 0040)	p. 87

XIVE

Xive

Implant: Ø 3	
Platform: 3 (Code 0084)	p. 113
Implant: Ø 3,4	
Platform: 3,4 (Code 0038)	p. 85
Implant: Ø 3,8	
Platform: 3,8 (Code 0039)	p. 86
Implant: Ø 4,5	
Platform: 4,5 (Code 0085)	p. 114
Implant: Ø 5,5	
Platform: 5,5 (Code 0086)	p. 115

YES IMPLANT

S-SYSTEM

Implant: Ø 3,3/3,5	
Platform: Narrow (Code 0030)	p. 81
Implant: Ø 4/4,5	
Platform: Regular (Code 0030)	p. 81
Implant: Ø 5/5,5	
Platform: Wide (Code 0030)	p. 81

ZACOM (OSSEOLIFE)

OEX

Implant: Ø 3,75/4,25	
Platform: RP 4,1 (Code 0024)	p. 75

ZIMMER

Eztec

Implant: Ø 3,1	
Platform: 2,9 (Code 0178)	p. 154

Screw-Vent

Implant: Ø 3,7/4,1	
Platform: 3,5 (Code 0040)	p. 87
Implant: Ø 4,7	
Platform: 4,5 (Code 0041)	p. 89
Implant: Ø 6	
Platform: 5,7 (Code 0080)	p. 109

Swiss-Plus

Implant: Ø 3,7/4,1/4,8	
Platform: 4,8 (Code 0074)	p. 107

Tapered Abutment Multi Unit

Implant: Ø Universal	
Platform: Universal (Code 0205)	p. 161

COMPATIBLE with 0001


STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
		0,3 mm				1,2 mm				mm				mm	
R	31.322.001.01-2	43°	25°	31.322.001.02-2	25°	-	-	-	-	-	-	-	-	-	-
NR	31.312.001.01-2			31.312.001.02-2											

DYNAMIC 3TIBASE®												
GINGIVAL HEIGHT		α_s	α_s	α_s								
		0,3 mm		CH=5mm	CH=7mm	CH=9mm						
R	31.322.001.21-2	25°	20°	10°								
NR	31.312.001.21-2											

DYNAMIC μ SCANBODY (LAB/CLIN)			DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL	SCANALOG				
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	α_{dp}	DYNAMIC MILLING TOOL	SHANK	α_{di}	SCANALOG
52.410.103.01-2	10			43.621.410.01-2			33.390.754.01-2	3		
				43.624.410.01-2			33.490.754.01-2	4	25°	
				43.630.410.01-2			33.690.754.01-2	6		
52.412.103.01-2	12									

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.20	ANALOG	LAB SCANBODY
41.316.084.01-2	-			43.618.201.01-2	18		
				43.624.201.01-2	24		
				43.632.201.01-2	32		

LIBRARY CODES											
STANDARD LIBRARY				CAPTIVE SCREW LIBRARY				LIBRARY OPTIONS			
LAB SCANBODY				LAB SCANBODY				GH = Gingival Height CH = Cement Height			
DYNAMIC μ SCANBODY (LAB/CLIN)				DYNAMIC μ SCANBODY (LAB/CLIN)				α_s = Standard maximum angulation α_c = Captive maximum angulation α_{di} = Direct to implant maximum angulation α_{dp} = Dynamic Premilled maximum angulation			
SCANALOG				SCANALOG				R = Rotational / Non-Engaging NR = Non Rotational / Engaging			

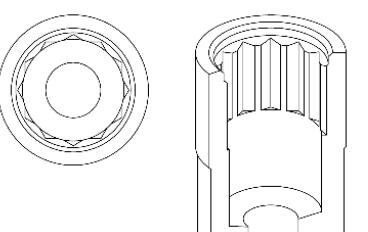

COMPATIBLE with 0002

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
		0,3 mm				1,2 mm				mm				mm	
R	31.323.002.01-2	45°	20°	31.323.002.02-2	25°	-	-	-	-	-	-	-	-	-	-
NR	31.313.002.01-2			31.313.002.02-2											

DYNAMIC 3TIBASE®												
GINGIVAL HEIGHT		α_s	α_s	α_s								
		0,3 mm		CH=5mm	CH=7mm	CH=9mm						
R	31.323.002.21-2	25°	20°	10°								
NR	31.313.002.21-2											

DYNAMIC μ SCANBODY (LAB/CLIN)			DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL	SCANALOG				
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	α_{dp}	DYNAMIC MILLING TOOL	SHANK	α_{di}	SCANALOG
52.408.101.01-2	8			43.621.410.01-2			33.390.805.01-2	3		
52.410.101.01-2	10			43.624.410.01-2			33.490.805.01-2	4	30°	
52.412.101.01-2	12			43.630.410.01-2			33.690.805.01-2	6		

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.20	ANALOG	LAB SCANBODY
41.316.084.01-2	-			43.618.201.01-2	18		
				43.624.201.01-2	24		
				43.632.201.01-2	32		

LIBRARY CODES				
---------------	--	--	--	--

COMPATIBLE with 0003

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
		mm				mm				mm				mm	
R	31.322.003.01-2	45°	30°	31.322.003.02-2	25°	-	-	-	-	-	-	-	-	-	-
NR	31.312.003.01-2			31.312.003.01-2											


DYNAMIC 3TIBASE®

GINGIVAL HEIGHT		
α_s	α_s	α_s
CH=5mm	CH= 7mm	CH= 9mm
R	-	-
NR	-	-

DYNAMIC µSCANBODY (LAB/CLIN)		DIGITAL ANALOG		DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL	
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	α_{dp}	DYNAMIC MILLING TOOL SHANK α_{di}
52.410.104.01-2	10		43.621.410.01-2				33.390.716.01-2 3
		50.312.003.01-2	43.624.410.01-2				33.490.716.01-2 4
52.412.104.01-2	12		43.630.410.01-2				33.690.716.01-2 6
				34.612.003.01-2			25°

DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.320.065.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

STRAIGHT SCREWS			
STRAIGHT SCREW	SCREWDRIVER Hex. 1.20	ANALOG	LAB SCANBODY
40.320.003.02-2	43.601.103.02-2	22.612.003.01-2	30.412.001.01-2

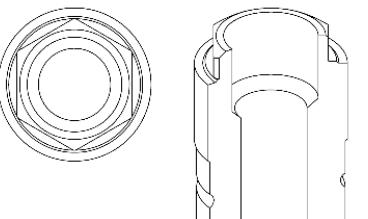

LIBRARY CODES

STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0003	LAB SCANBODY	DAS_C_E_0003
DYNAMIC µSCANBODY (LAB/CLIN)	DAS_I_10_0003	DYNAMIC µSCANBODY (LAB/CLIN)	DAS_C_I_10_0003
	DAS_I_12_0003		DAS_C_I_12_0003

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

COMPATIBLE with 0004

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
		mm				mm				mm				mm	
R	31.323.004.01-2	45°	29°	31.323.004.02-2	30°	20°	-	-	-	-	-	-	-	-	-
NR	31.313.004.01-2			31.313.004.02-2											

DYNAMIC 3TIBASE®

GINGIVAL HEIGHT		
α_s	α_s	α_s
1 mm	CH=5mm	CH=7mm
		CH=9mm
R	-	-
NR	-	-

DYNAMIC µSCANBODY (LAB/CLIN)		DIGITAL ANALOG		DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		SCANLOG
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	α_{dp}	DYNAMIC MILLING TOOL SHANK α_{di}	
52.410.103.01-2	10		50.313.004.01-2	43.620.411.01-2			33.390.754.01-2 3	
		50.313.004.03-2	43.624.410.01-2				33.490.754.01-2 4	
52.412.103.01-2	12		43.630.410.01-2				33.690.754.01-2 6	
				34.613.004.01-2 (1) 34.613.004.02-2 (2)				


DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.316.076.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

STRAIGHT SCREWS			
STRAIGHT SCREW	SCREWDRIVER Hex. 1.27	ANALOG	LAB SCANBODY
40.316.005.02-2	43.601.105.01-2	22.613.004.01-2	30.413.002.01-2

LIBRARY CODES

STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0004	LAB SCANBODY	DAS_C_E_0004
DYNAMIC µSCANBODY (LAB/CLIN)	DAS_I_10_0004	DYNAMIC µSCANBODY (LAB/CLIN)	DAS_C_I_10_0004
	DAS_I_12_0004		DAS_C_I_12_0004
SCANLOG	DAS_SA_0004	SCANLOG	DAS_C_SA_0004

LIBRARY OPTIONS			
GH	CH	IG	
Gingival Height	Cement Height	Adaptor 3mm	
α_s	α_c	α_{di}	α_{dp}
Standard maximum angulation	Captive maximum angulation	Direct to implant maximum angulation	Dynamic Premilled maximum angulation
R = Rotational / Non-Engaging			
NR = Non Rotational / Engaging			

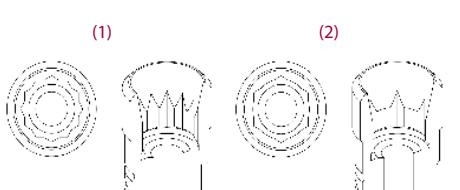

COMPATIBLE with 0005

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
1 mm		2 mm		mm		mm		mm		mm		mm		mm	
R	31.324.005.01-2	38°	23°	31.324.005.02-2	25°	15°	-	-	-	-	-	-	-	-	-
NR	31.314.005.01-2			31.314.005.02-2			-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®

GINGIVAL HEIGHT				
α_s	α_s	α_s		
1 mm	CH=5mm	CH=7mm	CH=9mm	
R	31.324.005.21-2	25°	20°	10°
NR	31.314.005.21-2			

DYNAMIC μSCANBODY (LAB/CLIN)

DIGITAL ANALOG

DYNAMIC PRE-MILLED

DYNAMIC MILLING TOOL

SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
52.410.102.01-2	10	50.314.005.01-2	43.620.411.01-2 43.621.410.01-2 43.624.410.01-2 43.630.410.01-2	34.614.005.01-2
		50.314.005.03-2	(IG=3mm)	
52.412.102.01-2	12			

COBALT-CHROME

α_{dp}

DYNAMIC MILLING TOOL

SHANK

α_{di}

33.390.958.01-2	3	30°
33.490.958.01-2	4	
33.690.958.01-2	6	

DYNAMIC SCREWS

DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.320.090.01-2	-	43.618.201.01-2 43.624.201.01-2 43.632.201.01-2	18 24 32

STRAIGHT SCREWS

STRAIGHT SCREW	SCREWDRIVER Hex. 1.27	ANALOG	LAB SCANBODY
40.320.005.03-2	43.601.105.01-2	22.614.005.01-2	30.413.002.01-2

LIBRARY CODES

STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0005	LAB SCANBODY	DAS_C_E_0005
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_L_10_0005 DAS_IG_10_0005	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_L_10_0005 DAS_C_IG_10_0005
	DAS_L_12_0005 DAS_IG_12_0005	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_L_12_0005 DAS_C_IG_12_0005

LIBRARY OPTIONS

GH = Gingival Height

CH = Cement Height

IG = Adaptor (3mm)

α_s = Standard maximum angulation


α_c = Captive maximum angulation

α_d = Direct to implant maximum angulation

α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging

NR = Non Rotational / Engaging

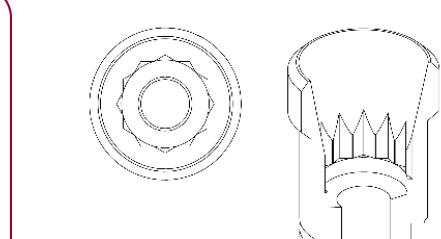

COMPATIBLE with 0006

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
1,2 mm				mm				mm				mm			
R	31.322.006.01-2	40°	20°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.312.006.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®

GINGIVAL HEIGHT			
α_s	α_s	α_s	
CH=5mm	CH=7mm	CH=9mm	
R	-	-	-
NR	-	-	-

DYNAMIC μSCANBODY (LAB/CLIN)

DIGITAL ANALOG

DYNAMIC PRE-MILLED

DYNAMIC MILLING TOOL

SCANALOG

SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
52.410.105.01-2	10	43.621.410.01-2 43.624.410.01-2 43.630.410.01-2	34.612.006.01-2	
		50.312.006.01-2		
52.412.105.01-2	12			

COBALT-CHROME

α_{dp}

DYNAMIC MILLING TOOL

SHANK

α_{di}

33.330.734.01-2	3	25°
33.430.734.01-2	4	
33.630.734.01-2	6	

DYNAMIC SCREWS

DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.316.072.01-2	-	43.618.201.01-2 43.624.201.01-2 43.632.201.01-2	18 24 32

STRAIGHT SCREWS

STRAIGHT SCREW	SCREWDRIVER Hex. 1.27	ANALOG	LAB SCANBODY
40.316.005.01-2	43.601.105.01-2	22.612.006.01-2	30.412.001.01-2

LIBRARY CODES

STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
------------------	--	-----------------------	--

COMPATIBLE with 0007

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
1,5 mm				mm				mm				mm			
R	31.323.007.01-2	38°	17°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.313.007.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®													
GINGIVAL HEIGHT		α_s	α_s	α_s									
1,5 mm		CH=5mm	CH=7mm	CH=9mm									
R	31.323.007.21-2	25°	20°	10°									
NR	31.313.007.21-2												

DYNAMIC μ SCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	α_{dp}	DYNAMIC MILLING TOOL SHANK	α_{di}
52.408.101.01-2	8			43.621.410.01-2				
52.410.101.01-2	10	50.313.007.01-2	43.624.410.01-2	34.613.007.01-2				
52.412.101.01-2	12		43.630.410.01-2		32.213.007.02-2	25°		

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.27	ANALOG	LAB SCANBODY
41.318.074.01-2	-			43.618.201.01-2	18		
				43.624.201.01-2	24		
				43.632.201.01-2	32		


LIBRARY CODES											
STANDARD LIBRARY				CAPTIVE SCREW LIBRARY				LIBRARY OPTIONS			
LAB SCANBODY	DAS_E_0007	LAB SCANBODY	DAS_C_E_0007	LAB SCANBODY	DAS_I_8_0007	DYNAMIC μ SCANBODY (LAB/CLIN)	DAS_L_8_0007	LAB SCANBODY	DAS_C_I_8_0007	DYNAMIC μ SCANBODY (LAB/CLIN)	DAS_C_L_8_0007
NR	31.313.007.01-2	R	31.323.007.01-2	R	31.323.007.21-2	NR	31.313.007.21-2	R	31.323.008.01-2	NR	31.313.008.01-2

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

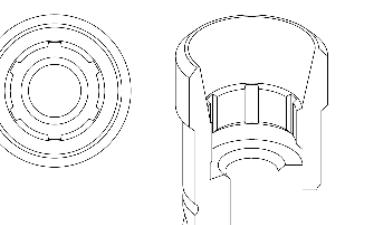

COMPATIBLE with 0008

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
0,5 mm				mm				mm				mm			
R	31.323.008.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	-			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®													
GINGIVAL HEIGHT		α_s	α_s	α_s									
0,5 mm		CH=5mm	CH=7mm	CH=9mm									
R	31.323.008.21-2	25°	20°	10°									
NR	-												

DYNAMIC μ SCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL	SCANALOG	
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	α_{dp}	DYNAMIC MILLING TOOL SHANK	α_{di}
52.408.113.01-2	8	50.313.008.01-2	43.621.410.01-2	43.624.410.01-2	34.613.008.01-2			
			43.630.410.01-2					

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.27	ANALOG	LAB SCANBODY
41.318.045.01-2	-			43.618.201.01-2	18		
				43.624.201.01-2	24		
				43.632.201.01-2	32		

LIBRARY CODES											
STANDARD LIBRARY											

COMPATIBLE with 0009

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
0,3 mm				0,5 mm				1 mm				mm			
R	31.322.009.01-2	45°	25°	31.322.009.02-2	25°	25°	31.322.009.03-2	25°	-	-	-	mm	-	-	-
NR	31.312.009.01-2			31.312.009.02-2			31.312.009.03-2					mm			

DYNAMIC 3TIBASE®			
GINGIVAL HEIGHT α_s α_s α_s			
CH=5mm CH=7mm CH=9mm			
R	-		
NR	-		

DYNAMIC µSCANBODY (LAB/CLIN)		DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
52.410.114.01-2	10		43.621.410.01-2	
		50.312.009.01-2	43.624.410.01-2	34.612.009.01-2
			43.630.410.01-2	
52.412.114.01-2	12			

DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.320.051.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

STRAIGHT SCREWS			
STRAIGHT SCREW	SCREWDRIVER Hex. 1.20	ANALOG	LAB SCANBODY
40.320.003.01-2	43.601.103.02-2	22.612.009.01-2	30.412.001.01-2


LIBRARY CODES	
STANDARD LIBRARY	
LAB SCANBODY	DAS_E_0009
DYNAMIC µSCANBODY (LAB/CLIN)	DAS_I_10_0009
	DAS_I_12_0009

CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_C_E_0009
DYNAMIC µSCANBODY (LAB/CLIN)	DAS_C_I_10_0009
	DAS_C_I_12_0009

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height

 α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

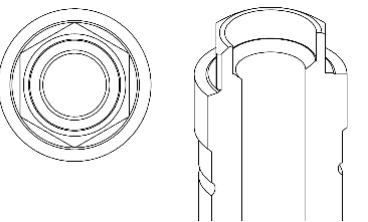

COMPATIBLE with 0010

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
0,3 mm		mm		mm		mm		mm		mm		mm		mm	
R	31.323.010.01-2	45°	29°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.313.010.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®			
GINGIVAL HEIGHT α_s α_s α_s			
CH=5mm CH=7mm CH=9mm			
R	-		
NR	-		

DYNAMIC µSCANBODY (LAB/CLIN)		DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
52.410.115.01-2	10		43.621.410.01-2	
		50.313.010.01-2	43.624.410.01-2	34.613.010.01-2
			43.630.410.01-2	
52.412.115.01-2	12			

DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.318.065.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

STRAIGHT SCREWS			
STRAIGHT SCREW	SCREWDRIVER Hex. 1.20	ANALOG	LAB SCANBODY
40.318.003.01-2	43.601.103.02-2	22.613.010.01-2	30.413.002.01-2


LIBRARY CODES	
STANDARD LIBRARY	
LAB SCANBODY	DAS_E_0010
DYNAMIC µSCANBODY (LAB/CLIN)	DAS_I_10_0010
	DAS_I_12_0010

CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_C_E_0010
DYNAMIC µSCANBODY (LAB/CLIN)	DAS_C_I_10_0010
	DAS_C_I_12_0010

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height

 α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

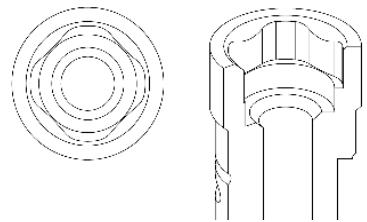

COMPATIBLE with 0011


STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
		mm				mm				mm				mm	
R	31.322.011.01-2	30°	29°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.312.011.01-2	-	-	-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®		
GINGIVAL HEIGHT		
α_s	α_s	α_s
CH=5mm	CH=7mm	CH=9mm
R	-	-
NR	-	-

DYNAMIC µSCANBODY (LAB/CLIN)		DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
52.410.108.01-2	10	50.312.011.01-2	43.621.410.01-2	34.612.011.01-2
			43.624.410.01-2	
			43.630.410.01-2	
52.412.108.01-2	12			

DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.316.094.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

STRAIGHT SCREWS			
STRAIGHT SCREW	SCREWDRIVER Hex. 1.27	ANALOG	LAB SCANBODY
40.316.005.04-2	43.601.105.01-2	-	30.412.001.01-2



LIBRARY CODES

STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0011	LAB SCANBODY	DAS_C_E_0011
DYNAMIC µSCANBODY (LAB/CLIN)	DAS_I_10_0011	DYNAMIC µSCANBODY (LAB/CLIN)	DAS_C_I_10_0011
	DAS_I_12_0011		DAS_C_I_12_0011

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

COMPATIBLE with 0012

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
		mm				mm				mm				mm	
R	31.323.012.01-2	33°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.313.012.01-2	-	-	-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®		
GINGIVAL HEIGHT		
α_s	α_s	α_s
CH=5mm	CH=7mm	CH=9mm
R	-	-
NR	-	-

DYNAMIC µSCANBODY (LAB/CLIN)		DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
52.410.109.01-2	10	50.313.012.01-2	43.621.410.01-2	34.613.012.01-2
			43.624.410.01-2	
			43.630.410.01-2	
52.412.109.01-2	12			

DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.316.094.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

STRAIGHT SCREWS			
STRAIGHT SCREW	SCREWDRIVER Hex. 1.27	ANALOG	LAB SCANBODY
40.316.005.04-2	43.601.105.01-2	-	30.413.002.01-2



LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0012	LAB SCANBODY	DAS_C_E_0012
DYNAMIC µSCANBODY (LAB/CLIN)	DAS_I_10_0012	DYNAMIC µSCANBODY (LAB/CLIN)	DAS_C_I_10_0012
	DAS_I_12_0012		DAS_C_I_12_0012

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

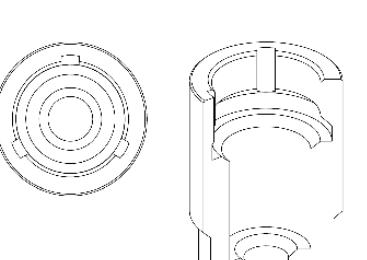

COMPATIBLE with 0013

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
		mm				mm				mm				mm	
R	31.323.013.01-2	43°	23°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.313.013.01-2	-	-	-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®		
GINGIVAL HEIGHT		
α_s	α_s	α_s
CH=5mm	CH=7mm	CH=9mm
R	-	-
NR	-	-

DYNAMIC µSCANBODY (LAB/CLIN)		DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
-	-	-	-	-
-	-	-	-	-

DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.320.074.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32


STRAIGHT SCREWS			
STRAIGHT SCREW	SCREWDRIVER TORX T6	ANALOG	LAB SCANBODY
40.320.007.02-2	43.601.107.01-2	-	30.413.002.01-2

LIBRARY CODES	
STANDARD LIBRARY	
LAB SCANBODY	DAS_E_0013
DYNAMIC µSCANBODY (LAB/CLIN)	-
CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_C_E_0013
DYNAMIC µSCANBODY (LAB/CLIN)	-

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height

 α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

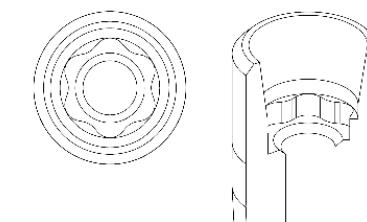

STANDARD DYNAMIC TIBASE®					
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT	
		1,2 mm		2 mm	
R	31.322.014.01-2	41°	23°	31.322.014.02-2	25°
NR	31.312.014.01-2	-	-	31.312.014.02-2	17°

DYNAMIC µSCANBODY (LAB/CLIN)					
DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL	SCANALOG		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME
52.410.128.01-2	10	-	43.620.411.01-2	-	-
		50.312.014.03-2	43.621.410.01-2	-	33.345.804.01-2
			43.624.410.01-2	-	33.445.804.01-2
			43.630.410.01-2	-	33.645.804.01-2
					25°
					23.412.014.01-2

DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.314.067.01-2	41.314.105.01-2	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32


STRAIGHT SCREWS			
STRAIGHT SCREW	SCREWDRIVER Hex. 1.20	ANALOG	LAB SCANBODY
40.314.003.04-2	43.601.103.02-2	-	30.412.001.01-2

LIBRARY CODES	
STANDARD LIBRARY	
LAB SCANBODY	DAS_E_0014
DYNAMIC µSCANBODY (LAB/CLIN)	DAS_I_10_0014
CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_C_E_0014
DYNAMIC µSCANBODY (LAB/CLIN)	DAS_C_I_10_0014
SCANALOG	DAS_SA_0014

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height
IG = Adaptor 3mm

 α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

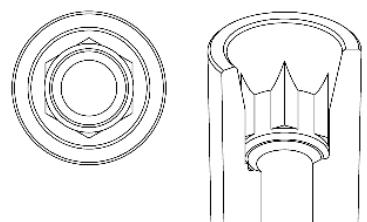

COMPATIBLE with 0015

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
1,7 mm		2,5 mm		mm		mm		mm		mm		mm		mm	
R	31.323.015.01-2	43°	23°	31.323.015.02-2	25°	15°	-	-	-	-	-	-	-	-	-
NR	31.313.015.01-2			31.313.015.02-2			-	-	-	-	-	-	-	-	-


DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α_s	α_s	α_s
1,7 mm		CH=5mm	CH=7mm	CH=9mm
R	31.323.015.21-2	30°	25°	10°
NR	31.313.015.21-2			

DYNAMIC μ SCANBODY (LAB/CLIN)			DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL	SCANALOG							
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	α_{dp}	DYNAMIC MILLING TOOL	SHANK	α_{di}	33.390.805.01-2	3	25°	23.413.015.01-2
52.410.104.01-2	10	50.313.015.01-2	43.621.410.01-2	34.613.015.01-2	-	-	33.390.805.01-2	3		33.490.805.01-2	4	25°	23.413.015.01-2
		50.313.015.03-2 (IG=3mm)	43.624.410.01-2				33.490.805.01-2	4		33.690.805.01-2	6		
52.412.104.01-2	12	50.313.015.03-2 (IG=3mm)	43.630.410.01-2				33.690.805.01-2	6					

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.20	ANALOG	LAB SCANBODY
41.318.080.01-2	-	43.618.201.01-2	18	40.318.003.02-2	43.601.103.02-2	-	30.413.002.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES	
STANDARD LIBRARY	
LAB SCANBODY	DAS_E_0015
DYNAMIC μ SCANBODY (LAB/CLIN)	DAS_L_10_0015 DAS_IG_10_0015 DAS_L_12_0015 DAS_IG_12_0015
SCANALOG	DAS_SA_0015
CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_C_E_0015
DYNAMIC μ SCANBODY (LAB/CLIN)	DAS_C_I_10_0015 DAS_C_IG_10_0015 DAS_C_I_12_0015 DAS_C_IG_12_0015
SCANALOG	DAS_C_SA_0015

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height
IG = Adaptador (3mm)
 α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_d = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation
R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

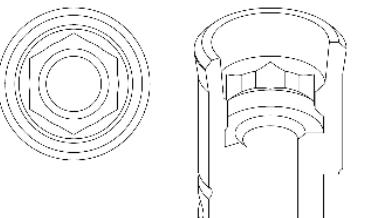

COMPATIBLE with 0016

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
0,8 mm				mm				mm				mm			
R	31.322.016.01-2	45°	28°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.312.016.01-2			-	-	-	-	-	-	-	-	-	-	-	-


DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α_s	α_s	α_s
CH=5mm		CH=7mm	CH=9mm	
R	-	-	-	-
NR	-	-	-	-

DYNAMIC μ SCANBODY (LAB/CLIN)			DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL	SCANALOG								
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	α_{dp}	DYNAMIC MILLING TOOL	SHANK	α_{di}	33.390.805.01-2	3	25°	23.413.015.01-2	
52.408.106.01-2	8													
52.410.106.01-2	10	50.312.016.01-2	43.621.410.01-2 43.624.410.01-2 43.630.410.01-2	34.612.016.01-2	-	-								
52.412.106.01-2	12													

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.27	ANALOG	LAB SCANBODY
41.316.071.01-2	-	43.618.201.01-2	18	40.316.005.05-2	43.601.105.01-2	-	30.412.001.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES	
STANDARD LIBRARY	
LAB SCANBODY	DAS_E_0016
DYNAMIC μ SCANBODY (LAB/CLIN)	DAS_I_8_0016 DAS_I_10_0016 DAS_I_12_0016
SCANALOG	DAS_I_12_0016
CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_C_E_0016
DYNAMIC μ SCANBODY (LAB/CLIN)	DAS_C_I_8_0016 DAS_C_I_10_0016 DAS_C_I_12_0016
SCANALOG	DAS_C_I_12_0016

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height
 α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_d = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation
R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

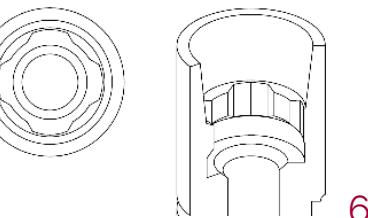

COMPATIBLE with 0017


STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
		mm				mm				mm				mm	
R	31.323.017.01-2	45°	24°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.313.017.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®											
GINGIVAL HEIGHT			α_s	α_s	α_s						
			CH=5mm	CH=7mm	CH=9mm						
R	31.323.017.21-2	30°	25°	15°							
NR	31.313.017.21-2										

DYNAMIC μ SCANBODY (LAB/CLIN)			DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL				
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	α_{dp}	DYNAMIC MILLING TOOL	SHANK	α_{di}
52.408.101.01-2	8			43.621.410.01-2			33.360.756.01-2	3	
52.410.101.01-2	10	50.313.017.01-2	43.624.410.01-2	34.613.017.01-2			33.460.756.01-2	4	30°
52.412.101.01-2	12		43.630.410.01-2				33.660.756.01-2	6	

DYNAMIC SCREWS				
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	
41.317.073.01-2	-		43.618.201.01-2	18
			43.624.201.01-2	24
			43.632.201.01-2	32

STRAIGHT SCREWS				
STRAIGHT SCREW	SCREWDRIVER Hex. 1.27	ANALOG	LAB SCANBODY	
40.317.005.01-2	43.601.105.01-2	-	30.413.002.01-2	



LIBRARY CODES

STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0017	LAB SCANBODY	DAS_C_E_0017
DYNAMIC μ SCANBODY (LAB/CLIN)	DAS_I_8_0017	DYNAMIC μ SCANBODY (LAB/CLIN)	DAS_C_I_8_0017
	DAS_I_10_0017		DAS_C_I_10_0017
	DAS_I_12_0017		DAS_C_I_12_0017

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

COMPATIBLE with 0018

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
		mm				mm				mm				mm	
R	31.324.018.01-2	39°	18°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.314.018.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®														
GINGIVAL HEIGHT			α_s	α_s	α_s									
			CH=5mm	CH=7mm	CH=9mm									
R	-		-	-	-									
NR	-		-	-	-									

DYNAMIC μ SCANBODY (LAB/CLIN)			DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL				
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	α_{dp}	DYNAMIC MILLING TOOL	SHANK	α_{di}
52.410.102.01-2	10			43.621.410.01-2			33.360.756.01-2	3	
		50.314.018.01-2	43.624.410.01-2	34.614.018.01-2			33.460.756.01-2	4	30°
52.412.102.01-2	12		43.630.410.01-2				33.660.756.01-2	6	

DYNAMIC SCREWS				
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	
41.317.073.01-2	-		43.618.201.01-2	18
			43.624.201.01-2	24
			43.632.201.01-2	32

STRAIGHT SCREWS				
STRAIGHT SCREW	SCREWDRIVER Hex. 1.27	ANALOG	LAB SCANBODY	
40.317.005.01-2	43.601.105.01-2	-	30.413.002.01-2	

LIBRARY CODES

STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0018	LAB SCANBODY	DAS_C_E_0018

</tbl

COMPATIBLE with 0019

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
		mm				mm				mm				mm	
R	31.322.019.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.312.019.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®

GINGIVAL HEIGHT		
α_s	α_s	α_s
CH=5mm	CH=7mm	CH=9mm
R	-	-
NR	-	-

DYNAMIC µSCANBODY (LAB/CLIN)

DIGITAL ANALOG

DYNAMIC PRE-MILLED

DYNAMIC MILLING TOOL


SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
52.410.105.01-2	10		43.621.410.01-2	
		50.312.019.01-2	43.624.410.01-2	34.612.019.01-2
52.412.105.01-2	12		43.630.410.01-2	

COBALT-CHROME	α_{dp}
-	-
-	25°
-	-

DYNAMIC MILLING TOOL	SHANK	α_{di}
33.360.754.01-2	3	
33.460.754.01-2	4	25°
33.660.754.01-2	6	

DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.316.071.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

STRAIGHT SCREWS		
STRAIGHT SCREW	SCREWDRIVER Hex. 1.27	ANALOG LAB SCANBODY
40.316.005.05-2	43.601.105.01-2	30.412.001.01-2

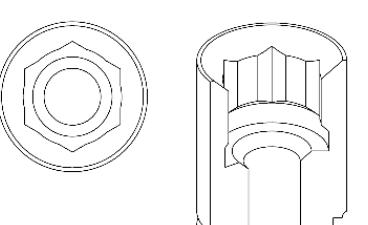

LIBRARY CODES

STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0019	LAB SCANBODY	DAS_C_E_0019
DYNAMIC µSCANBODY (LAB/CLIN)	DAS_I_10_0019	DYNAMIC µSCANBODY (LAB/CLIN)	DAS_C_I_10_0019
	DAS_I_12_0019		DAS_C_I_12_0019

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

COMPATIBLE with 0020

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
		mm				mm				mm				mm	
R	31.323.020.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	-			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®

GINGIVAL HEIGHT		
α_s	α_s	α_s
CH=5mm	CH=7mm	CH=9mm
R	-	-
NR	-	-

DYNAMIC µSCANBODY (LAB/CLIN)

DIGITAL ANALOG

DYNAMIC PRE-MILLED

DYNAMIC MILLING TOOL

SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
52.408.112.01-2	8			
-	10	50.313.020.01-2	43.620.411.01-2	34.613.020.01-2
-	12			

COBALT-CHROME	α_{dp}
-	-
-	25°
-	-

DYNAMIC MILLING TOOL	SHANK	α_{di}
33.390.716.01-2	3	
33.490.716.01-2	4	30°
33.690.716.01-2	6	

DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.316.044.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32


STRAIGHT SCREWS		
STRAIGHT SCREW	SCREWDRIVER Hex. 1.27	ANALOG LAB SCANBODY
40.316.005.06-2	43.601.105.01-2	30.413.005.01-2

LIBRARY CODES

STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0020	LAB SCANBODY	DAS_C_E_0020
DYNAMIC µSCANBODY (LAB/CLIN)	DAS_I_8_0020	DYNAMIC µSCANBODY (LAB/CLIN)	DAS_C_I_8_0020

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height
 α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

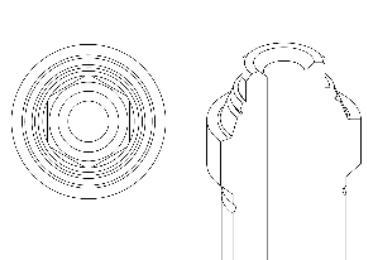

COMPATIBLE with 0023

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
		0,3 mm		0,5 mm				mm		mm		mm		mm	
R	31.322.023.01-2	45°	30°	31.322.023.02-2	25°	30°	-	-	-	-	-	-	-	-	-
NR	31.312.023.01-2			31.312.023.02-2			-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®

GINGIVAL HEIGHT			α_s	α_s	α_s
CH=5mm	CH= 7mm	CH= 9mm			
R	-				
NR	-				

DYNAMIC µSCANBODY (LAB/CLIN)

DIGITAL ANALOG		DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		SCANALOG	
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	α_{dp}	DYNAMIC MILLING TOOL SHANK α_{di}
52.410.103.01-2	10		43.621.410.01-2				33.390.805.01-2 3
		50.312.023.01-2	43.624.410.01-2				33.490.805.01-2 4
52.412.103.01-2	12		43.630.410.01-2				33.690.805.01-2 6

DYNAMIC SCREWS

DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.316.059.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

STRAIGHT SCREW	SCREWDRIVER UNIGRIP	ANALOG	LAB SCANBODY
40.316.008.01-2	43.601.108.01-2	22.612.023.01-2	30.412.001.01-2

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0023	LAB SCANBODY	DAS_C_E_0023
DYNAMIC µSCANBODY (LAB/CLIN)	DAS_I_10_0023	DYNAMIC µSCANBODY (LAB/CLIN)	DAS_C_I_10_0023
SCANALOG	DAS_SA_0023	SCANALOG	DAS_C_SA_0023

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

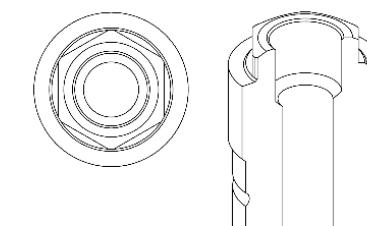

COMPATIBLE with 0024

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
		0,3 mm		0,5 mm				mm		mm		mm		mm	
R	31.323.024.01-2	45°	30°	31.323.024.02-2	30°	30°	-	-	-	-	-	-	-	-	-
NR	31.313.024.01-2			31.313.024.02-2			-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®

GINGIVAL HEIGHT			α_s	α_s	α_s	GINGIVAL HEIGHT			α_s	α_s	α_s	GINGIVAL HEIGHT			α_s	α_s	α_s		
0,3 mm	CH=5mm	CH= 7mm	CH= 9mm	0,5 mm	CH=5mm	CH=7mm	CH=9mm	1 mm	CH=5mm	CH=7mm	CH=9mm	2 mm	CH=5mm	CH=7mm	CH=9mm	2 mm	CH=5mm	CH=7mm	CH=9mm
R	31.323.024.21-2	30°	25°	10°	31.323.024.22-2	30°	25°	10°	31.323.024.23-2	30°	25°	10°	31.323.024.24-2	30°	25°	10°			
NR	31.313.024.21-2				31.313.024.22-2				31.313.024.23-2				31.313.024.24-2						

DYNAMIC µSCANBODY (LAB/CLIN)

DIGITAL ANALOG		DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		SCANALOG	
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	α_{dp}	DYNAMIC MILLING TOOL SHANK α_{di}
52.408.101.01-2	8			43.621.410.01-2			33.390.716.01-2 3
52.410.101.01-2	10			43.624.410.01-2			33.490.716.01-2 4
52.412.101.01-2	12			43.630.410.01-2			33.690.716.01-2 6

DYNAMIC SCREWS

DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.320.060.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

STRAIGHT SCREW	SCREWDRIVER UNIGRIP	ANALOG	LAB SCANBODY
40.320.008.01-2	43.601.108.01-2	22.613.024.01-2	30.413.002.01-2

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0024	LAB SCANBODY	DAS_C_E_0024
DYNAMIC µSCANBODY (LAB/CLIN)	DAS_I_8_0024	DYNAMIC µSCANBODY (LAB/CLIN)	DAS_C_I_8_0024
SCANALOG	DAS_SA_0024	SCANALOG	DAS_C_SA_0024

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

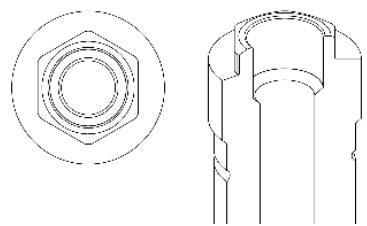

COMPATIBLE with 0025

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
0,3 mm		0,5 mm		mm		mm		mm		mm		mm		mm	
R	31.323.025.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	-	-	-	-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®

GINGIVAL HEIGHT				
α_s	α_s	α_s		
0,3 mm	CH=5mm	CH=7mm	CH=9mm	
R	31.323.025.21-2	30°	25°	10°
NR	-	-	-	-

DYNAMIC μ SCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL	SCANALOG	
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	α_{dp}	DYNAMIC MILLING TOOL SHANK	α_{di}
52.408.112.01-2	8	50.313.025.02-2	43.620.411.01-2	34.613.025.01-2	-	-	33.390.716.01-2	3
52.410.111.01-2	10	50.313.025.01-2	43.621.410.01-2 43.624.410.01-2 43.630.410.01-2	-	-	-	33.490.716.01-2	4

DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.314.039.01-2	-	43.618.201.01-2 43.624.201.01-2 43.632.201.01-2	18 24 32


LIBRARY CODES	
STANDARD LIBRARY	
LAB SCANBODY	DAS_E_0025
DYNAMIC μ SCANBODY (LAB/CLIN)	DAS_I_8_0025 DAS_I_10_0025
SCANALOG	DAS_SA_0025

CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_C_E_0025
DYNAMIC μ SCANBODY (LAB/CLIN)	DAS_C_I_8_0025 DAS_C_I_10_0025
SCANALOG	DAS_C_SA_0025

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height

 α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

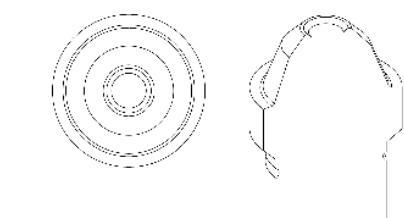

COMPATIBLE with 0026

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
0,5 mm		1,2 mm		mm		mm		mm		mm		mm		mm	
R	31.322.026.01-2	45°	29°	31.322.026.02-2	25°	22°	-	-	-	-	-	-	-	-	-
NR	31.312.026.01-2	-	-	31.312.026.02-2	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®

GINGIVAL HEIGHT				
α_s	α_s	α_s		
0,5 mm	CH=5mm	CH=7mm	CH=9mm	
R	31.322.026.21-2	25°	20°	10°
NR	31.312.026.21-2	-	-	-

DYNAMIC μ SCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL	SCANALOG	
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	α_{dp}	DYNAMIC MILLING TOOL SHANK	α_{di}
52.410.108.01-2	10	50.312.026.01-2	43.621.410.01-2 43.624.410.01-2 43.630.410.01-2	34.612.026.01-2	-	-	33.390.805.01-2	3
52.412.108.01-2	12	-	-	-	-	-	33.490.805.01-2	4

DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.318.075.01-2	-	43.618.201.01-2 43.624.201.01-2 43.632.201.01-2	18 24 32


LIBRARY CODES	
STANDARD LIBRARY	
LAB SCANBODY	DAS_E_0026
DYNAMIC μ SCANBODY (LAB/CLIN)	DAS_I_10_0026 DAS_I_12_0026
SCANALOG	DAS_SA_0026

CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_C_E_0026
DYNAMIC μ SCANBODY (LAB/CLIN)	DAS_C_I_10_0026 DAS_C_I_12_0026
SCANALOG	DAS_C_SA_0026

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height

 α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

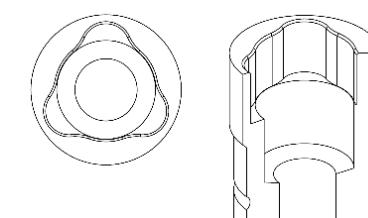

COMPATIBLE with 0027


STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
		0,3 mm				1,2 mm				mm				mm	
R	31.323.027.01-2	39°	29°	31.323.027.02-2	25°	22°	-	-	-	-	-	-	-	-	-
NR	31.313.027.01-2			31.313.027.02-2			-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α_s	α_s	α_s
0,3 mm		CH=5mm	CH=7mm	CH=9mm
R	31.323.027.21-2	25°	20°	10°
NR	31.313.027.21-2			

DYNAMIC μ SCANBODY (LAB/CLIN)		DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
52.410.109.01-2	10		43.621.410.01-2	
		50.313.027.01-2	43.624.410.01-2	34.613.027.01-2
52.412.109.01-2	12		43.630.410.01-2	

DYNAMIC SCREWS				
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	
41.320.090.01-2	-	43.618.201.01-2	18	
		43.624.201.01-2	24	
		43.632.201.01-2	32	

STRAIGHT SCREWS				
STRAIGHT SCREW	SCREWDRIVER UNIGRIP	ANALOG	LAB SCANBODY	
40.320.008.03-2	43.601.108.01-2	22.613.027.01-2	30.413.002.01-2	




LIBRARY CODES	
STANDARD LIBRARY	
LAB SCANBODY	DAS_E_0027
DYNAMIC μ SCANBODY (LAB/CLIN)	DAS_I_10_0027
	DAS_I_12_0027

CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_C_E_0027
DYNAMIC μ SCANBODY (LAB/CLIN)	DAS_C_I_10_0027
	DAS_C_I_12_0027

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height

 α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging



COMPATIBLE with 0028

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
		0,3 mm				mm				mm				mm	
R	31.324.028.01-2	38°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.314.028.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α_s	α_s	α_s
CH=5mm		CH=7mm	CH=9mm	
R	-		-	-
NR	-		-	-


DYNAMIC μ SCANBODY (LAB/CLIN)		DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
52.410.109.01-2	10		43.621.410.01-2	
		50.314.028.01-2	43.624.410.01-2	34.614.028.01-2
52.412.109.01-2	12		43.630.410.01-2	

DYNAMIC SCREWS				
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	
41.320.090.01-2	-	43.618.201.01-2	18	
		43.624.201.01-2	24	
		43.632.201.01-2	32	

STRAIGHT SCREWS				
STRAIGHT SCREW	SCREWDRIVER UNIGRIP	ANALOG	LAB SCANBODY	
40.320.008.03-2	43.601.108.01-2	22.614.028.01-2	30.413.002.01-2	

LIBRARY CODES	
STANDARD LIBRARY	
LAB SCANBODY	DAS_E_0028
DYNAMIC μ SCANBODY (LAB/CLIN)	DAS_I_10_0028
	DAS_I_12_0028

CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_C_E_0028
DYNAMIC μ SCANBODY (LAB/CLIN)	DAS_C_I_10_0028
	DAS_C_I_12_0028

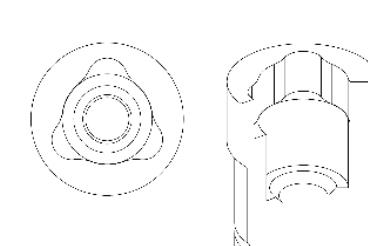

COMPATIBLE with 0029

STANDARD DYNAMIC TIBASE®																							
GINGIVAL HEIGHT			α_s		GINGIVAL HEIGHT			α_s		GINGIVAL HEIGHT													
1,2 mm			2 mm		mm			4 mm		mm													
R	31.322.029.01-2	37°	23°	31.322.029.02-2	25°	15°	-	-	31.322.029.04-2	15°	25°	-	-	31.322.029.04-2	15°	30°	31.323.030.04-2	15°	30°	-	-	-	-
NR	31.312.029.01-2			31.312.029.02-2			-	-	31.312.029.04-2			-	-				31.313.030.04-2			-	-		

DYNAMIC 3TIBASE®			
GINGIVAL HEIGHT			
	α_s	α_s	α_s
	CH=5mm	CH=7mm	CH=9mm
R	-	-	-
NR	-	-	-


DYNAMIC µSCANBODY (LAB/CLIN)			DIGITAL ANALOG		DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		SCANALOG	
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	α_{dp}	DYNAMIC MILLING TOOL	SHANK	α_{di}	
52.410.103.01-2	10	50.312.029.01-2	43.621.410.01-2	34.613.029.01-2			33.345.804.01-2	3		
		50.312.029.03-2	43.624.410.01-2				33.445.804.01-2	4	20°	23.412.029.01-2
52.412.103.01-2	12	(IG=3mm)	43.630.410.01-2				33.645.804.01-2	6		

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.20	ANALOG	LAB SCANBODY
41.316.094.01-2	41.316.132.01-2		43.618.201.01-2	18			
			43.624.201.01-2	24			
			43.632.201.01-2	32			

LIBRARY CODES	
STANDARD LIBRARY	
LAB SCANBODY	DAS_E_0029
DYNAMIC µSCANBODY (LAB/CLIN)	DAS_L_10_0029 DAS_C_IG_10_0029 DAS_I_12_0029 DAS_C_IG_12_0029
SCANALOG	DAS_SA_0029

CAPTIVE SCREW LIBRARY	
LIBRARY OPTIONS	
LAB SCANBODY	DAS_C_E_0029
DYNAMIC µSCANBODY (LAB/CLIN)	DAS_C_I_10_0029 DAS_C_IG_10_0029 DAS_C_I_12_0029 DAS_C_IG_12_0029
SCANALOG	DAS_C_SA_0029

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height
IG = Adaptor (3mm)
 α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation
R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

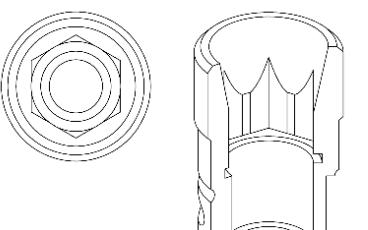

COMPATIBLE with 0030

STANDARD DYNAMIC TIBASE®												
GINGIVAL HEIGHT			α_s		GINGIVAL HEIGHT			α_s		GINGIVAL HEIGHT		
1,1 mm			2 mm		mm			3 mm		4 mm		
R	31.323.030.01-2	42°	25°	31.323.030.02-2	25°	15°	31.323.030.03-2	20°	30°	31.323.030.04-2	15°	30°
NR	31.313.030.01-2			31.313.030.02-2			31.313.030.03-2			31.313.030.04-2		

DYNAMIC 3TIBASE®			
GINGIVAL HEIGHT			
	α_s	α_s	α_s
	CH=5mm	CH=7mm	CH=9mm
R	-	-	-
NR	-	-	-


DYNAMIC µSCANBODY (LAB/CLIN)			DIGITAL ANALOG		DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		SCANALOG	
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	α_{dp}	DYNAMIC MILLING TOOL	SHANK	α_{di}	
52.408.101.01-2	8	50.313.030.01-2	43.621.410.01-2	34.613.030.01-2			33.345.808.01-2	3		
52.410.101.01-2	10	50.313.030.03-2	43.624.410.01-2				33.445.808.01-2	4		
52.412.101.01-2	12	(IG=3mm)	43.630.410.01-2				33.645.808.01-2	6		

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.20	ANALOG	LAB SCANBODY
41.320.079.01-2	41.320.125.01-2		43.618.201.01-2	18			
			43.624.201.01-2	24			
			43.632.201.01-2	32			

LIBRARY CODES	
STANDARD LIBRARY	
LAB SCANBODY	DAS_E_0030
DYNAMIC µSCANBODY (LAB/CLIN)	DAS_L_10_0030 DAS_C_IG_10_0030 DAS_I_12_0030 DAS_C_IG_12_0030
SCANALOG	DAS_SA_0030

CAPTIVE SCREW LIBRARY	
LIBRARY OPTIONS	
LAB SCANBODY	DAS_C_E_0030
DYNAMIC µSCANBODY (LAB/CLIN)	DAS_C_I_10_0030 DAS_C_IG_10_0030 DAS_C_I_12_0030 DAS_C_IG_12_0030
SCANALOG	DAS_C_SA_0030

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height
IG = Adaptor (3mm)
 α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation
R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

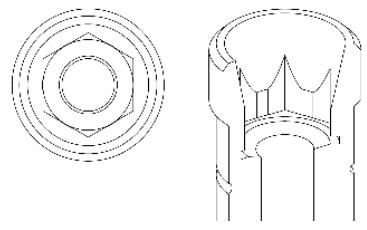

COMPATIBLE with 0033


STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
1,3 mm		2 mm		mm		mm		mm		mm		mm		mm	
R	31.322.033.01-2	38°	18°	31.322.033.02-2	20°	14°	-	-	-	-	-	-	-	-	-
NR	31.312.033.01-2			31.312.033.02-2			-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α_s	α_s	α_s
1,3 mm		CH=5mm	CH=7mm	CH=9mm
R	31.322.033.21-2	25°	20°	10°
NR	31.312.033.21-2			

DYNAMIC µSCANBODY (LAB/CLIN)			DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL				
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	α_{dp}	DYNAMIC MILLING TOOL	SHANK	α_{di}
52.408.106.01-2	8	50.312.033.01-2	43.621.410.01-2	34.612.033.01-2	32.212.033.02-2	25°	33.315.804.01-2	3	
52.410.106.01-2	10	50.312.033.03-2	43.624.410.01-2	43.630.410.01-2			33.415.804.01-2	4	25°
52.412.106.01-2	12	(IG=3mm)	43.624.410.01-2	43.630.410.01-2			33.615.804.01-2	6	

DYNAMIC SCREWS				
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	
41.316.078.01-2	41.316.124.01-2	43.618.201.01-2	18	
		43.624.201.01-2	24	
		43.632.201.01-2	32	

STRAIGHT SCREWS			
STRAIGHT SCREW	SCREWDRIVER TORX T6	ANALOG	LAB SCANBODY
40.316.007.01-2	43.601.107.01-2	22.612.033.01-2	30.412.001.01-2



LIBRARY CODES

STANDARD LIBRARY	
LAB SCANBODY	DAS_E_0033
DYNAMIC µSCANBODY (LAB/CLIN)	DAS_I_8_0033 DAS_C_I_8_0033 DAS_I_10_0033 DAS_C_I_10_0033 DAS_I_12_0033 DAS_C_I_12_0033
	DAS_C_I_8_0033 DAS_C_I_10_0033 DAS_C_I_12_0033
	DAS_C_I_10_0033 DAS_C_I_12_0033

CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_C_E_0033
DYNAMIC µSCANBODY (LAB/CLIN)	DAS_C_I_8_0033 DAS_C_I_10_0033 DAS_C_I_12_0033 DAS_C_I_12_0033

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height
IG = Adaptor (3mm)
 α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_d = Direct to implant maximum angulation
 α_{di} = Dynamic Premilled maximum angulation
R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

COMPATIBLE with 0035

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
1,1 mm		2 mm		3 mm		4 mm		mm		mm		mm		mm	
R	31.323.035.01-2	39°	18°	31.323.035.02-2	20°	14°	-	-	-	-	-	-	-	-	-
NR	31.313.035.01-2			31.313.035.02-2			-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT		α_s	α_s	α_s
1,1 mm		CH=5mm	CH=7mm	CH=9mm
R	31.323.035.21-2	25°	20°	10°
NR	31.313.035.21-2			


DYNAMIC µSCANBODY (LAB/CLIN)			DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL	SCANALOG			
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	α_{dp}	DYNAMIC MILLING TOOL	SHANK	α_{di}
52.410.107.01-2	10	50.313.035.01-2	43.621.410.01-2	34.613.035.01-2	32.213.035.02-2	25°	33.315.804.01-2	3	
		50.313.035.03-2	43.624.410.01-2	43.630.410.01-2			33.415.804.01-2	4	25°
52.412.107.01-2	12	(IG=3mm)	43.624.410.01-2	43.630.410.01-2			33.615.804.01-2	6	

DYNAMIC SCREWS				
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	
41.316.078.01-2	41.316.124.01-2	43.618.201.01-2	18	
		43.624.201.01-2	24	
		43.632.201.01-2	32	

STRAIGHT SCREWS			
STRAIGHT SCREW	SCREWDRIVER TORX T6	ANALOG	LAB SCANBODY
40.316.007.01-2	43.601.107.01-2	22.613.035.01-2	30.413.002.01-2

LIBRARY CODES	
STANDARD LIBRARY	CAPTIVE SCREW LIBRARY
LAB SCANBODY	DAS_E_0035
DYNAMIC µSCANBODY (LAB/CLIN)	DAS_I_10_0035 DAS_C_I_10_0035 DAS_I_12_0035 DAS_C_I_12_0035
SCANALOG	DAS_SA_0035

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height
IG = Adaptor (3mm)
 α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_d = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation
R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

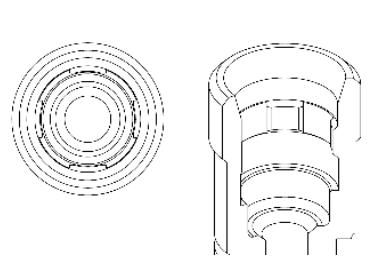

COMPATIBLE with 0037

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
		mm				mm				mm				mm	
R	31.323.037.01-2	45°	25°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.313.037.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®			
GINGIVAL HEIGHT α_s α_s α_s			
CH=5mm CH=7mm CH=9mm			
R	-	-	-
NR	-	-	-

DYNAMIC µSCANBODY (LAB/CLIN)		DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
52.410.110.01-2	10	50.313.037.01-2	43.621.410.01-2	34.613.037.01-2
			43.624.410.01-2	
			43.630.410.01-2	
52.412.110.01-2	12			

COBALT-CHROME	α_{dp}	DYNAMIC MILLING TOOL	SHANK	α_{di}
32.213.037.02-2	30°	33.315.708.01-2	3	30°
		33.415.708.01-2	4	
		33.615.708.01-2	6	

DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.320.067.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32


STRAIGHT SCREW	SCREWDRIVER TORX T6	ANALOG	LAB SCANBODY
40.320.007.01-2	43.601.107.01-2	22.613.037.01-2	30.413.004.01-2

LIBRARY CODES	
STANDARD LIBRARY	
LAB SCANBODY	DAS_E_0037
DYNAMIC µSCANBODY (LAB/CLIN)	DAS_I_10_0037
	DAS_I_12_0037
CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_C_E_0037
DYNAMIC µSCANBODY (LAB/CLIN)	DAS_C_I_10_0037
	DAS_C_I_12_0037

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

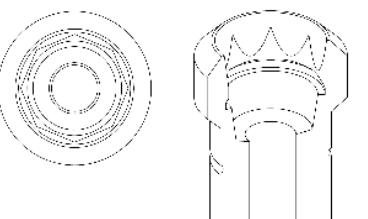

COMPATIBLE with 0038

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
		mm				mm				mm				mm	
R	31.322.038.01-2	45°	29°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.312.038.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®			
GINGIVAL HEIGHT α_s α_s α_s			
0,7 mm CH=5mm CH=7mm CH=9mm			
R	31.322.038.21-2	30°	25°
NR	31.312.038.21-2		10°

DYNAMIC µSCANBODY (LAB/CLIN)		DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
52.410.103.01-2	10	50.312.038.01-2	43.621.410.01-2	34.612.038.01-2
			43.624.410.01-2	
			43.630.410.01-2	
52.412.103.01-2	12			

COBALT-CHROME	α_{dp}	DYNAMIC MILLING TOOL	SHANK	α_{di}
		33.316.081.01-2	3	30°
		43.624.201.01-2	4	
		43.632.201.01-2	6	

DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.316.081.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32


STRAIGHT SCREW	SCREWDRIVER Hex. 1.25	ANALOG	LAB SCANBODY
40.316.004.02-2	43.601.104.01-2	-	30.412.001.01-2

LIBRARY CODES	
STANDARD LIBRARY	
LAB SCANBODY	DAS_E_0038
DYNAMIC µSCANBODY (LAB/CLIN)	DAS_I_10_0038
	DAS_I_12_0038
CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_C_E_0038
DYNAMIC µSCANBODY (LAB/CLIN)	DAS_C_I_10_0038
	DAS_C_I_12_0038

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

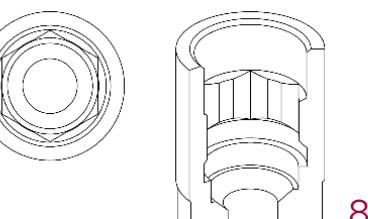

COMPATIBLE with 0039

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
0,7 mm				mm				mm				mm			
R	31.323.039.01-2	45°	29°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.313.039.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®

GINGIVAL HEIGHT			
α_s	α_s	α_s	
0,7 mm	CH=5mm	CH= 7mm	CH= 9mm
R	31.323.039.21-2	30°	25°
NR	31.313.039.21-2		10°

DYNAMIC µSCANBODY (LAB/CLIN)

DIGITAL ANALOG

DYNAMIC PRE-MILLED

DYNAMIC MILLING TOOL

SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
52.410.114.01-2	10		43.621.410.01-2	
		50.313.039.01-2	43.624.410.01-2	34.613.039.01-2
52.412.114.01-2	12		43.630.410.01-2	

COBALT-CHROME	α_{dp}
-	-
-	-
-	-

DYNAMIC MILLING TOOL	SHANK	α_{di}
33.345.856.01-2	3	
33.445.856.01-2	4	25°
33.645.856.01-2	6	

DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.316.081.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

STRAIGHT SCREWS	SCREWDRIVER Hex. 1.25	ANALOG	LAB SCANBODY
40.316.004.02-2	43.601.104.01-2	-	30.413.002.01-2
		-	
		-	

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0039	LAB SCANBODY	DAS_C_E_0039
DYNAMIC µSCANBODY (LAB/CLIN)	DAS_L_10_0039	DYNAMIC µSCANBODY (LAB/CLIN)	DAS_C_L_10_0039
	DAS_L_12_0039		DAS_C_L_12_0039

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

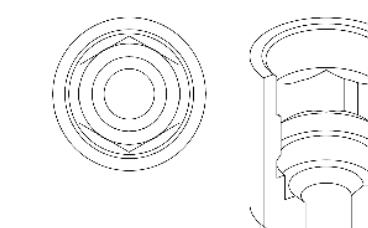

COMPATIBLE with 0040

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
0,6 mm				1,5 mm				3 mm				4 mm			
R	31.322.040.01-2	45°	30°	31.322.040.02-2	25°	25°	20°	31.322.040.03-2	20°	30°	15°	31.322.040.04-2	15°	30°	10°
NR	31.312.040.01-2			31.312.040.02-2				31.312.040.03-2				31.312.040.04-2			23°
NR (Friction-Fit)	31.312.042.01-2														

DYNAMIC 3TIBASE®

GINGIVAL HEIGHT			
α_s	α_s	α_s	
0,6 mm	CH=5mm	CH= 7mm	CH= 9mm
R	31.322.040.21-2	25°	20°
NR	31.312.040.21-2		10°

DYNAMIC µSCANBODY (LAB/CLIN)

DIGITAL ANALOG

DYNAMIC PRE-MILLED

DYNAMIC MILLING TOOL

SCANLOG

SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
52.408.101.01-2	8		43.621.410.01-2	
52.410.101.01-2	10	50.312.040.01-2	43.624.410.01-2	34.612.040.01-2
52.412.101.01-2	12	50.312.040.03-2 (IG=3mm)	43.630.410.01-2	

DYNAMIC SCREWS

STRAIGHT SCREWS

DYNAMIC SCREWDRIVER

SCREWDRIVER LENGTH (mm)

DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.317.071.01-2	41.317.106.01-2	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

STRAIGHT SCREWS

SCREWDRIVER

Hex. 1.27

ANALOG	LAB SCANBODY
40.317.004.01-2	43.601.104.01-2
22.612.040.01-2	30.412.001.01-2

LIBRARY CODES

STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0040	LAB SCANBODY	DAS_C_E_0040
DYNAMIC µSCANBODY (LAB/CLIN)	DAS_L_10_0040	DYNAMIC µSCANBODY (LAB/CLIN)	DAS_C_L_10_0040
	DAS_L_12_0040		DAS_C_L_12_0040
SCANLOG	DAS_SA_0040	SCANLOG	DAS_C_SA_0040

LIBRARY OPTIONS

COMPATIBLE with 0040b

STANDARD DYNAMIC TIBASE®																																		
GINGIVAL HEIGHT			α_s		α_c		GINGIVAL HEIGHT			α_s		α_c		GINGIVAL HEIGHT			α_s		α_c		GINGIVAL HEIGHT			α_s		α_c								
0,6 mm							1,5 mm							3 mm							mm							5 mm						
R	31.322.040.01-2		45°	30°	31.322.040.02-2		25°	25°	31.322.040.03-2	20°	30°	-	-	31.322.040.05-2		10°	25°																	
NR	31.312.040.01-2				31.312.040.02-2				31.312.040.03-2			-	-	31.312.040.05-2																				

DYNAMIC 3TIBASE®

GINGIVAL HEIGHT				α_s	α_s	α_s
0,6 mm				CH=5mm	CH=7mm	CH=9mm
R	31.322.040.21-2		25°	20°	10°	
NR	31.312.040.21-2					

DYNAMIC μSCANBODY (LAB/CLIN)

SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
-	-			
-	-	-	-	
-	-			-

DYNAMIC SCREWS

DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.318.071.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0040	LAB SCANBODY	DAS_C_E_0040
DYNAMIC μSCANBODY (LAB/CLIN)	-	DYNAMIC μSCANBODY (LAB/CLIN)	-

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

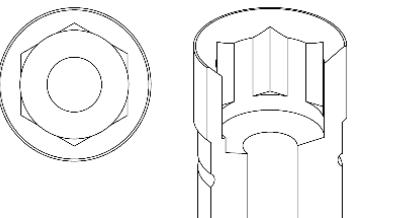

COMPATIBLE with 0041

STANDARD DYNAMIC TIBASE®																														
GINGIVAL HEIGHT			α_s		α_c		GINGIVAL HEIGHT			α_s		α_c		GINGIVAL HEIGHT			α_s		α_c		GINGIVAL HEIGHT			α_s		α_c				
0,4 mm							1,5 mm							mm							mm									
R	31.323.041.01-2		45°	30°	31.323.041.02-2		30°	25°	-	-	-	-	-	-	-	-	-	-	-	-	-	-	-	-	-	-	-	-		
NR	31.313.041.01-2				31.313.041.02-2																									
NR (Friction-Fit)	31.313.043.01-2																													

DYNAMIC 3TIBASE®

GINGIVAL HEIGHT				α_s	α_s	α_s
0,4 mm				CH=5mm	CH=7mm	CH=9mm
R	31.323.041.21-2		30°	20°	10°	
NR	31.313.041.21-2					

DYNAMIC μSCANBODY (LAB/CLIN)

SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
52.410.102.01-2	10		50.313.041.01-2	43.621.410.01-2
			50.313.041.03-2	43.624.410.01-2
52.412.102.01-2	12		43.630.410.01-2	34.613.041.01-2

DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.317.071.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0041	LAB SCANBODY	DAS_C_E_0041
DYNAMIC μSCANBODY (LAB/CLIN)	-	DYNAMIC μSCANBODY (LAB/CLIN)	-
SCANALOG	DAS_SA_0041	SCANALOG	DAS_C_SA_0041

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height
IG = Adaptor (3mm)

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

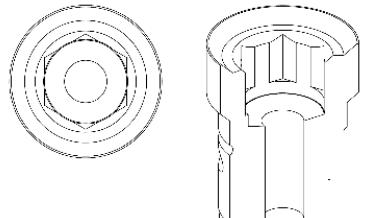

COMPATIBLE with 0041b

STANDARD DYNAMIC TIBASE®												
	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
	0,4 mm		1,5 mm		mm		mm		mm		mm	
R	31.323.041.01-2		45°	30°	31.323.041.02-2		30°	25°	-	-	-	-
NR	31.313.041.01-2				31.313.041.02-2				-	-	-	-

DYNAMIC 3TIBASE®			
	GINGIVAL HEIGHT	α_s	α_s
	0,4 mm	CH=5mm	CH=7mm
R	31.323.041.21-2		30°
NR	31.313.041.21-2		20°
			10°

DYNAMIC μ SCANBODY (LAB/CLIN)		DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
-	-			
-	-			

COBALT-CHROME	α_{dp}	DYNAMIC MILLING TOOL	SHANK	α_{di}
32.013.041.02-2	30°	33.370.716.01-2	3	
		33.470.716.01-2	4	30°
		33.670.716.01-2	6	

DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.318.071.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32


STRAIGHT SCREW	SCREWDRIVER Hex. 1.27	ANALOG	LAB SCANBODY
-			30.413.002.01-2

LIBRARY CODES	
STANDARD LIBRARY	
LAB SCANBODY	DAS_E_0041
DYNAMIC μ SCANBODY (LAB/CLIN)	-
CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_C_E_0041
DYNAMIC μ SCANBODY (LAB/CLIN)	-

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height

 α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

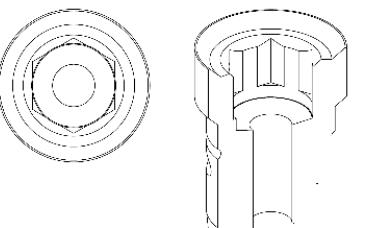

COMPATIBLE with 0044

STANDARD DYNAMIC TIBASE®												
	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
	1 mm		mm	mm	mm		mm	mm	mm		mm	mm
R	31.322.044.01-2		42°	23°	-	-	-	-	-	-	-	-
NR	31.312.044.01-2				-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®			
	GINGIVAL HEIGHT	α_s	α_s
	1 mm	CH=5mm	CH=7mm
R	31.322.044.21-2		25°
NR	-		20°
			10°

DYNAMIC μ SCANBODY (LAB/CLIN)		DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
52.410.105.01-2	10		43.621.410.01-2	
			43.624.410.01-2	
			43.630.410.01-2	
50.312.044.01-2				
52.412.105.01-2	12			

DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.318.065.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32


STRAIGHT SCREW	SCREWDRIVER Hex. 1.27	ANALOG	LAB SCANBODY
-			30.412.001.01-2

LIBRARY CODES	
STANDARD LIBRARY	
LAB SCANBODY	DAS_E_0044
DYNAMIC μ SCANBODY (LAB/CLIN)	DAS_I_10_0044
CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_C_E_0044
DYNAMIC μ SCANBODY (LAB/CLIN)	DAS_C_I_10_0044
	DAS_C_I_12_0044

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height

 α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

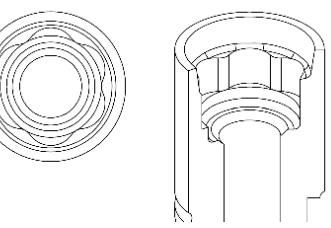

COMPATIBLE with 0045

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
1 mm		mm		mm		mm		mm		mm		mm		mm	
R	31.323.045.01-2	43°	22°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.313.045.01-2	-	-	-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®

GINGIVAL HEIGHT				
α_s	α_s	α_s		
1 mm	CH=5mm	CH=7mm	CH=9mm	
R	31.323.045.21-2	30°	20°	10°
NR	31.313.045.21-2	-	-	-

DYNAMIC µSCANBODY (LAB/CLIN)

SCANBODY		HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
52.410.118.01-2	10			43.621.410.01-2	
			50.313.045.01-2	43.624.410.01-2	34.613.045.01-2
				43.630.410.01-2	

DYNAMIC SCREWS

DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.318.065.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0045	LAB SCANBODY	DAS_C_E_0045
DYNAMIC µSCANBODY (LAB/CLIN)	DAS_I_10_0045	DYNAMIC µSCANBODY (LAB/CLIN)	DAS_C_I_10_0045
	DAS_I_12_0045		DAS_C_I_12_0045

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

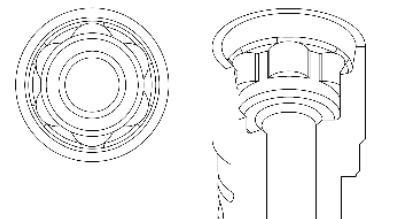

COMPATIBLE with 0046

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
1 mm		mm		mm		mm		mm		mm		mm		mm	
R	31.324.046.01-2	42°	21°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.314.046.01-2	-	-	-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®

GINGIVAL HEIGHT				
α_s	α_s	α_s		
1 mm	CH=5mm	CH=7mm	CH=9mm	
R	31.324.046.21-2	30°	20°	10°
NR	-	-	-	-

DYNAMIC µSCANBODY (LAB/CLIN)

SCANBODY		HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
52.410.125.01-2	10			43.621.410.01-2	
			50.314.046.01-2	43.624.410.01-2	34.614.046.01-2
				43.630.410.01-2	

DYNAMIC SCREWS

DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.318.065.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0046	LAB SCANBODY	DAS_C_E_0046
DYNAMIC µSCANBODY (LAB/CLIN)	DAS_I_10_0046	DYNAMIC µSCANBODY (LAB/CLIN)	DAS_C_I_10_0046
	DAS_I_12_0046		DAS_C_I_12_0046

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

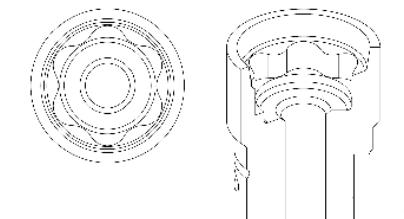

COMPATIBLE with 0047

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
		0,6 mm				mm				mm				mm	
R	31.322.047.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.312.047.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®		
GINGIVAL HEIGHT		
α_s	α_s	α_s
CH=5mm	CH=7mm	CH=9mm
R	-	-
NR	-	-


DYNAMIC µSCANBODY (LAB/CLIN)		DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
52.410.123.01-2	10		43.621.410.01-2	
		50.312.047.01-2	43.624.410.01-2	34.612.047.01-2
			43.630.410.01-2	
52.412.123.01-2	12			

DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.320.074.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

STRAIGHT SCREWS			
STRAIGHT SCREW	SCREWDRIVER TORX T6	ANALOG	LAB SCANBODY
40.320.007.02-2	43.601.107.01-2	-	30.412.001.01-2

LIBRARY CODES	
STANDARD LIBRARY	
LAB SCANBODY	DAS_E_0047
DYNAMIC µSCANBODY (LAB/CLIN)	DAS_I_10_0047
	DAS_I_12_0047
CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_C_E_0047
DYNAMIC µSCANBODY (LAB/CLIN)	DAS_C_I_10_0047
	DAS_C_I_12_0047

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height
 α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation
R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

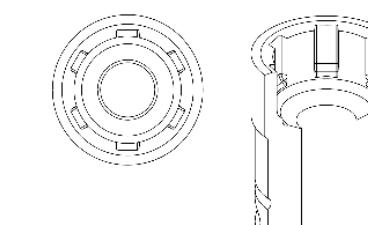

COMPATIBLE with 0048

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
		0,6 mm				mm				mm				mm	
R	31.323.048.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.313.048.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®		
GINGIVAL HEIGHT		
α_s	α_s	α_s
CH=5mm	CH=7mm	CH=9mm
R	-	-
NR	-	-


DYNAMIC µSCANBODY (LAB/CLIN)		DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
52.410.123.01-2	10		43.621.410.01-2	
		50.312.047.01-2	43.624.410.01-2	34.612.047.01-2
			43.630.410.01-2	
52.412.123.01-2	12			

DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.320.074.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

STRAIGHT SCREWS			
STRAIGHT SCREW	SCREWDRIVER TORX T6	ANALOG	LAB SCANBODY
40.320.007.02-2	43.601.107.01-2	-	30.413.002.01-2

LIBRARY CODES	
STANDARD LIBRARY	
LAB SCANBODY	DAS_E_0048
DYNAMIC µSCANBODY (LAB/CLIN)	DAS_I_10_0048
	DAS_I_12_0048
CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_C_E_0048
DYNAMIC µSCANBODY (LAB/CLIN)	DAS_C_I_10_0048
	DAS_C_I_12_0048

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height
 α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation
R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

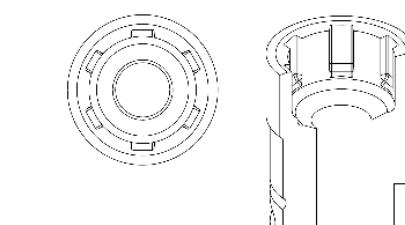

COMPATIBLE with 0049

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
		mm				mm				mm				mm	
R	31.321.049.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.311.049.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®

GINGIVAL HEIGHT		
α_s	α_s	α_s
CH=5mm	CH=7mm	CH=9mm
R	-	-
NR	-	-

DYNAMIC μ SCANBODY (LAB/CLIN)

DIGITAL ANALOG

DYNAMIC PRE-MILLED

DYNAMIC MILLING TOOL


SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
52.410.116.01-2	10		43.621.410.01-2	34.611.049.01-2
		50.311.049.01-2	43.624.410.01-2	
52.412.116.01-2	12		43.630.410.01-2	

COBALT-CHROME	α_{dp}
-	-
-	25°
-	-

DYNAMIC MILLING TOOL	SHANK	α_{di}
33.325.472.01-2	3	
33.425.472.01-2	4	25°
33.625.472.01-2	6	

DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.314.064.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

STRAIGHT SCREWS		
STRAIGHT SCREW	SCREWDRIVER Hex. 1.25	ANALOG LAB SCANBODY
40.314.004.01-2	43.601.104.01-2	30.412.001.01-2

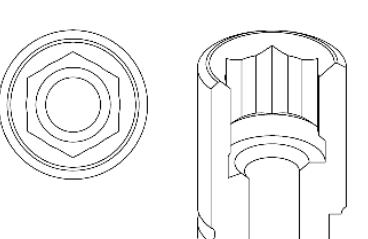

LIBRARY OPTIONS

GH = Gingival Height

CH = Cement Height

α_s = Standard maximum angulation

α_c = Captive maximum angulation

α_{di} = Direct to implant maximum angulation

α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging

NR = Non Rotational / Engaging

COMPATIBLE with 0050

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
		mm				mm				mm				mm	
R	31.323.051.01-2	45°	27°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.313.051.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®

GINGIVAL HEIGHT		
α_s	α_s	α_s
CH=5mm	CH=7mm	CH=9mm
R	-	-
NR	-	-

DYNAMIC μ SCANBODY (LAB/CLIN)

DIGITAL ANALOG

DYNAMIC PRE-MILLED

DYNAMIC MILLING TOOL

SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
52.410.117.01-2	10		43.621.410.01-2	34.612.050.01-2
		50.312.050.01-2	43.624.410.01-2	
52.412.117.01-2	12		43.630.410.01-2	

COBALT-CHROME	α_{dp}
-	-
-	25°
-	-

DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.318.064.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

STRAIGHT SCREWS		
STRAIGHT SCREW	SCREWDRIVER Hex. 1.25	ANALOG LAB SCANBODY
40.318.004.03-2	43.601.104.01-2	30.412.001.01-2

LIBRARY CODES

STANDARD LIBRARY	
LAB SCANBODY	DAS_E_0050
DYNAMIC μ SCANBODY (LAB/CLIN)	DAS_I_10_0050
	DAS_I_12_0050
DYNAMIC μ SCANBODY (LAB/CLIN)	DAS_C_E_0050
DYNAMIC μ SCANBODY (LAB/CLIN)	DAS_C_I_10_0050
DYNAMIC μ SCANBODY (LAB/CLIN)	DAS_C_I_12_0050

CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_C_E_0050
DYNAMIC μ SCANBODY (LAB/CLIN)	DAS_C_I_10_0050
DYNAMIC μ SCANBODY (LAB/CLIN)	DAS_C_I_12_0050

LIBRARY OPTIONS	
GH = Gingival Height	CH = Cement Height
α_s = Standard maximum angulation	
α_c = Captive maximum angulation	
α_{di} = Direct to implant maximum angulation	
α_{dp} = Dynamic Premilled maximum angulation	

COMPATIBLE with 0051

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
		0,5 mm				mm				mm				mm	
R	31.323.051.01-2	45°	25°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.313.051.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®		
GINGIVAL HEIGHT		
α_s	α_s	α_s
CH=5mm	CH=7mm	CH=9mm
R	-	-
NR	-	-

DYNAMIC µSCANBODY (LAB/CLIN)		DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
52.410.118.01-2	10		43.621.410.01-2	34.613.051.01-2
		50.313.051.01-2	43.624.410.01-2	
			43.630.410.01-2	
52.412.118.01-2	12			

DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.318.064.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32


STRAIGHT SCREWS		
STRAIGHT SCREW	SCREWDRIVER Hex. 1.25	ANALOG LAB SCANBODY
40.318.004.03-2	43.601.104.01-2	30.412.001.01-2

LIBRARY CODES	
STANDARD LIBRARY	
LAB SCANBODY	DAS_E_0051
DYNAMIC µSCANBODY (LAB/CLIN)	DAS_I_10_0051
	DAS_I_12_0051
CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_C_E_0051
DYNAMIC µSCANBODY (LAB/CLIN)	DAS_C_I_10_0051
	DAS_C_I_12_0051

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height

 α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

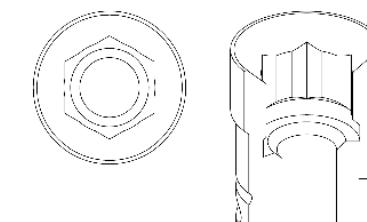

COMPATIBLE with 0052

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
		0,3 mm				mm				mm				mm	
R	31.324.052.01-2	45°	27°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.314.052.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®		
GINGIVAL HEIGHT		
α_s	α_s	α_s
CH=5mm	CH=7mm	CH=9mm
R	-	-
NR	-	-

DYNAMIC µSCANBODY (LAB/CLIN)		DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
52.410.102.01-2	10		43.621.410.01-2	34.614.052.01-2
		50.314.052.01-2	43.624.410.01-2	
			43.630.410.01-2	
52.412.102.01-2	12			

DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.318.064.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32


STRAIGHT SCREWS		
STRAIGHT SCREW	SCREWDRIVER Hex. 1.25	ANALOG LAB SCANBODY
40.318.004.03-2	43.601.104.01-2	30.413.002.01-2

LIBRARY CODES	
STANDARD LIBRARY	
LAB SCANBODY	DAS_E_0052
DYNAMIC µSCANBODY (LAB/CLIN)	DAS_I_10_0052
	DAS_I_12_0052
CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_C_E_0052
DYNAMIC µSCANBODY (LAB/CLIN)	DAS_C_I_10_0052
	DAS_C_I_12_0052

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height

 α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

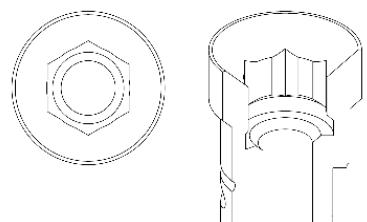

COMPATIBLE with 0054


STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
	mm			mm			mm			mm					
R	31.323.054.01-2	45°	25°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.313.054.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®		
GINGIVAL HEIGHT		
α_s	α_s	α_s
CH=5mm	CH= 7mm	CH= 9mm
R	-	-
NR	-	-

DYNAMIC μ SCANBODY (LAB/CLIN)		DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL	
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	
52.410.119.01-2	10	50.314.054.01-2	43.621.410.01-2	34.614.054.01-2	
			43.624.410.01-2		
			43.630.410.01-2		
52.412.119.01-2	12				

DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.318.067.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

STRAIGHT SCREWS		
STRAIGHT SCREW	SCREWDRIVER	-
ANALOG	LAB SCANBODY	
40.318.012.01-2	-	30.413.002.01-2



LIBRARY CODES

STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0054	LAB SCANBODY	DAS_C_E_0054
DYNAMIC μ SCANBODY (LAB/CLIN)	DAS_L_10_0054	DYNAMIC μ SCANBODY (LAB/CLIN)	DAS_C_L_10_0054
	DAS_L_12_0054		DAS_C_L_12_0054

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

COMPATIBLE with 0057

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
	mm			mm			mm			mm					
R	31.324.057.01-2	45°	27°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.314.057.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®		
GINGIVAL HEIGHT		
α_s	α_s	α_s
CH=5mm	CH= 7mm	CH= 9mm
R	-	-
NR	-	-

DYNAMIC μ SCANBODY (LAB/CLIN)		DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
52.408.101.01-2	8	50.314.057.01-2	43.621.410.01-2	34.614.057.01-2
52.410.101.01-2	10		43.624.410.01-2	
52.412.101.01-2	12		43.630.410.01-2	

DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.316.084.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

STRAIGHT SCREWS		
STRAIGHT SCREW	SCREWDRIVER	-
ANALOG	LAB SCANBODY	
40.316.003.01-2	43.601.103.02-2	

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0057	LAB SCANBODY	DAS_C_E_0057
DYNAMIC μ SCANBODY (LAB/CLIN)	DAS_L_8_0057	DYNAMIC μ SCANBODY (LAB/CLIN)	DAS_C_L_8_0057
	DAS_L_10_0057		DAS_C_L_10_0057
	DAS_L_12_0057		DAS_C_L_12_0057

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

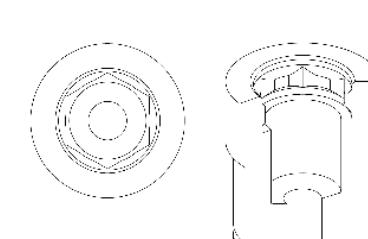

COMPATIBLE with 0058

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
0,5 mm				mm				mm				mm			
R	31.324.058.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.314.058.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®		
GINGIVAL HEIGHT		
α_s	α_s	α_s
CH=5mm	CH=7mm	CH=9mm
R	-	-
NR	-	-

DYNAMIC µSCANBODY (LAB/CLIN)		DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
52.410.118.01-2	10	50.314.058.01-2	43.621.410.01-2	34.614.058.01-2
			43.624.410.01-2	
			43.630.410.01-2	
52.412.118.01-2	12			

DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.320.047.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

STRAIGHT SCREWS			
STRAIGHT SCREW	SCREWDRIVER Hex. 1.20	ANALOG	LAB SCANBODY
40.320.003.01-2	43.601.103.02-2	22.614.058.01-2	30.414.003.01-2


LIBRARY CODES	
STANDARD LIBRARY	
LAB SCANBODY	DAS_E_0058
DYNAMIC µSCANBODY (LAB/CLIN)	DAS_I_10_0058
	DAS_I_12_0058

CAPTIVE SCREW LIBRARY	
STANDARD LIBRARY	
LAB SCANBODY	DAS_C_E_0058
DYNAMIC µSCANBODY (LAB/CLIN)	DAS_C_I_10_0058
	DAS_C_I_12_0058

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

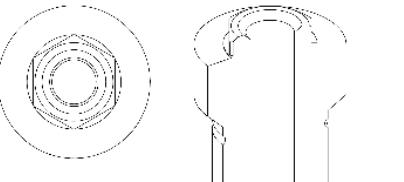

COMPATIBLE with 0059

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
0,7 mm															
R	31.324.059.01-2	45°	27°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.314.059.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®		
GINGIVAL HEIGHT		
α_s	α_s	α_s
CH=5mm	CH=7mm	CH=9mm
R	-	-
NR	-	-

DYNAMIC µSCANBODY (LAB/CLIN)		DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
-	-	-	-	-
-	-	-	-	-
-	-	-	-	-

DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.318.065.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

STRAIGHT SCREWS			
STRAIGHT SCREW	SCREWDRIVER Hex. 1.20	ANALOG	LAB SCANBODY
40.318.003.01-2	43.601.103.02-2	22.614.059.01-2	30.414.003.01-2


LIBRARY CODES	
STANDARD LIBRARY	
LAB SCANBODY	DAS_E_0059
DYNAMIC µSCANBODY (LAB/CLIN)	-
	-

CAPTIVE SCREW LIBRARY	
STANDARD LIBRARY	
LAB SCANBODY	DAS_C_E_0059
DYNAMIC µSCANBODY (LAB/CLIN)	-
	-

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

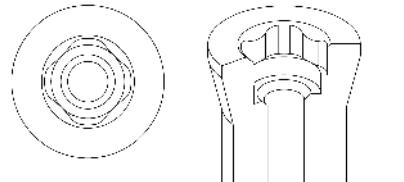

COMPATIBLE with 0060

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
		mm				mm				mm				mm	
R	31.324.060.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.314.060.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®														
GINGIVAL HEIGHT			α_s	α_s	α_s	CH=5mm			CH=7mm			CH=9mm		
R	-	-	-	-	-									
NR	-	-	-	-	-									

DYNAMIC µSCANBODY (LAB/CLIN)		DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL					
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	α_{dp}	DYNAMIC MILLING TOOL	SHANK	α_{di}
52.410.122.01-2	10		50.314.060.01-2	43.621.410.01-2 43.624.410.01-2 43.630.410.01-2	34.614.060.01-2		33.390.716.01-2 33.490.716.01-2 33.690.716.01-2	3	
								4	30°
52.412.122.01-2	12							6	


DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.20	ANALOG	LAB SCANBODY
41.320.060.01-2	-			43.618.201.01-2 43.624.201.01-2 43.632.201.01-2	18 24 32	40.320.003.02-2 43.601.103.02-2	22.614.060.01-2 30.415.007.01-2

LIBRARY CODES											
STANDARD LIBRARY				CAPTIVE SCREW LIBRARY				LIBRARY OPTIONS			
LAB SCANBODY				LAB SCANBODY				GH = Gingival Height CH = Cement Height			
DYNAMIC µSCANBODY (LAB/CLIN)				DYNAMIC µSCANBODY (LAB/CLIN)				α_s = Standard maximum angulation α_c = Captive maximum angulation α_{di} = Direct to implant maximum angulation α_{dp} = Dynamic Premilled maximum angulation			
DAS_E_0060				DAS_C_E_0060				α_s	α_c	α_{di}	α_{dp}
DAS_I_10_0060				DAS_C_I_10_0060							
DAS_I_12_0060				DAS_C_I_12_0060							

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

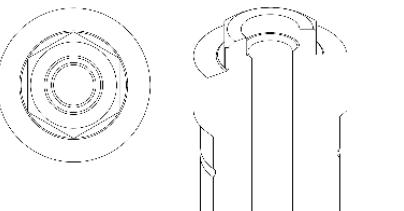

COMPATIBLE with 0061

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
		mm				mm				mm				mm	
R	31.324.061.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.314.061.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®														
GINGIVAL HEIGHT			α_s	α_s	α_s	CH=5mm			CH=7mm			CH=9mm		
R	-	-	-	-	-									
NR	-	-	-	-	-									

DYNAMIC µSCANBODY (LAB/CLIN)		DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL					
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	α_{dp}	DYNAMIC MILLING TOOL	SHANK	α_{di}
52.410.125.01-2	10		50.314.061.01-2	43.621.410.01-2 43.624.410.01-2 43.630.410.01-2	34.614.061.01-2		33.390.958.01-2 33.490.958.01-2 33.690.958.01-2	3	
								4	30°
52.412.125.01-2	12							6	

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER UNIGRIP	ANALOG	LAB SCANBODY
41.325.067.01-2	-			43.618.201.01-2 43.624.201.01-2 43.632.201.01-2	18 24 32	40.325.008.01-2 43.601.108.01-2	22.614.061.01-2 30.415.007.01-2

LIBRARY CODES											
STANDARD LIBRARY				CAPTIVE SCREW LIBRARY				LIBRARY OPTIONS			
LAB SCANBODY											

COMPATIBLE with 0066

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
		mm				mm				mm				mm	
R	31.323.066.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	-	-	-	-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®		
GINGIVAL HEIGHT		
α_s	α_s	α_s
CH=5mm	CH=7mm	CH=9mm
R	-	-
NR	-	-

DYNAMIC µSCANBODY (LAB/CLIN)		DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
-	-	-	-	-
-	-	-	-	-
-	-	-	-	-

DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.314.039.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

STRAIGHT SCREWS			
STRAIGHT SCREW	SCREWDRIVER	-	ANALOG LAB SCANBODY
-	-	-	22.613.066.01-2 30.412.001.01-2


LIBRARY CODES

STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0066	LAB SCANBODY	DAS_C_E_0066
DYNAMIC µSCANBODY (LAB/CLIN)	-	DYNAMIC µSCANBODY (LAB/CLIN)	-

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

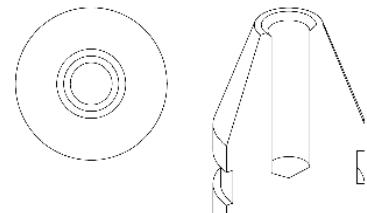

COMPATIBLE with 0074

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
	mm			mm			mm			mm					
R	31.323.074.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.313.074.01-2	-	-	-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®		
GINGIVAL HEIGHT		
α_s	α_s	α_s
CH=5mm	CH=7mm	CH=9mm
R	-	-
NR	-	-

DYNAMIC µSCANBODY (LAB/CLIN)		DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL	SCANALOG
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME
52.410.110.01-2	10		43.621.410.01-2		
		50.313.074.01-2	43.624.410.01-2	34.613.074.01-2	
52.412.110.01-2	12		43.630.410.01-2		

DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.320.044.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

STRAIGHT SCREWS			
STRAIGHT SCREW	SCREWDRIVER	-	ANALOG LAB SCANBODY
40.320.007.04-2	43.601.102.01-2	-	22.613.074.01-2 30.415.007.01-2


LIBRARY CODES

STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0074	LAB SCANBODY	DAS_C_E_0074
DYNAMIC µSCANBODY (LAB/CLIN)	-	DYNAMIC µSCANBODY (LAB/CLIN)	-
		DAS_C_I_10_0074	
		DAS_C_I_12_0074	
		SCANALOG	DAS_C_SA_0074

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

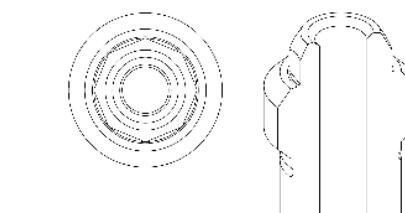

COMPATIBLE with 0075


STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
1 mm		2 mm		mm		mm		mm		mm		mm		mm	
R	31.322.075.01-2	42°	24°	31.322.075.02-2	25°	15°	-	-	-	-	-	-	-	-	-
NR	-	-	-	-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®		
GINGIVAL HEIGHT		
α_s	α_s	α_s
CH=5mm	CH=7mm	CH=9mm
R	-	-
NR	-	-

DYNAMIC µSCANBODY (LAB/CLIN)		DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL	
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	
52.410.105.01-2	10	50.312.075.01-2	43.621.410.01-2	34.612.075.01-2	
			43.624.410.01-2		
			43.630.410.01-2		
52.412.105.01-2	12				

DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.318.077.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

STRAIGHT SCREWS			
STRAIGHT SCREW	SCREWDRIVER Hex. 1.00	ANALOG	LAB SCANBODY
40.318.013.01-2	-	22.612.075.01-2	30.412.001.01-2



LIBRARY CODES

STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0075	LAB SCANBODY	DAS_C_E_0075
DYNAMIC µSCANBODY (LAB/CLIN)	DAS_I_10_0075	DYNAMIC µSCANBODY (LAB/CLIN)	DAS_C_I_10_0075
	DAS_I_12_0075		DAS_C_I_12_0075

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

COMPATIBLE with 0080

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
0,4 mm		mm		mm		mm		mm		mm		mm		mm	
R	31.324.080.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.314.080.01-2	-	-	-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®		
GINGIVAL HEIGHT		
α_s	α_s	α_s
CH=5mm	CH=7mm	CH=9mm
R	-	-
NR	-	-

DYNAMIC µSCANBODY (LAB/CLIN)		DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
52.410.124.01-2	10	50.314.080.01-2	43.621.410.01-2	34.614.080.01-2
			43.624.410.01-2	
			43.630.410.01-2	
52.412.124.01-2	12			

DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.317.071.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

STRAIGHT SCREWS			
STRAIGHT SCREW	SCREWDRIVER Hex. 1.27	ANALOG	LAB SCANBODY
40.317.004.01-2	43.601.104.01-2	22.614.080.01-2	30.414.003.01-2

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0080	LAB SCANBODY	DAS_C_E_0080
DYNAMIC µSCANBODY (LAB/CLIN)	DAS_I_10_0080	DYNAMIC µSCANBODY (LAB/CLIN)	DAS_C_I_10_0080
	DAS_I_12_0080		DAS_C_I_12_0080

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

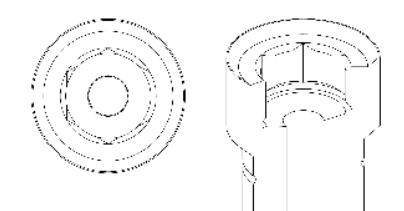

COMPATIBLE with 0081

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
		mm				mm				mm				mm	
R	31.325.081.01-2	41°	18°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.315.081.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®

GINGIVAL HEIGHT		
α_s	α_s	α_s
CH=5mm	CH=7mm	CH=9mm
R	-	-
NR	-	-

DYNAMIC µSCANBODY (LAB/CLIN)

SCANBODY		HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
52.410.126.01-2	10		50.315.081.01-2	43.621.410.01-2 43.624.410.01-2 43.630.410.01-2	34.615.081.01-2
52.412.126.01-2	12				

DYNAMIC SCREWS

DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.318.064.01-2	-	43.618.201.01-2 43.624.201.01-2 43.632.201.01-2	18 24 32

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0081	LAB SCANBODY	DAS_C_E_0081
DYNAMIC µSCANBODY (LAB/CLIN)	DAS_I_10_0081 DAS_I_12_0081	DYNAMIC µSCANBODY (LAB/CLIN)	DAS_C_I_10_0081 DAS_C_I_12_0081

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

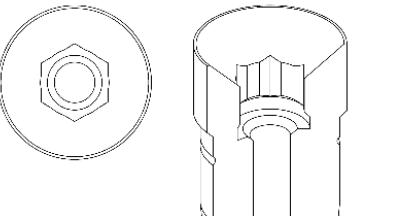

COMPATIBLE with 0082

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
		mm				mm				mm				mm	
R	31.322.082.01-2	45°	25°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.312.082.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®

GINGIVAL HEIGHT		
α_s	α_s	α_s
CH=5mm	CH=7mm	CH=9mm
R	-	-
NR	-	-

DYNAMIC µSCANBODY (LAB/CLIN)

SCANBODY		HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
52.410.105.01-2	10		50.312.082.01-2	43.621.410.01-2 43.624.410.01-2 43.630.410.01-2	34.612.082.01-2
52.412.105.01-2	12				

DYNAMIC SCREWS

DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.316.074.01-2	-	43.618.201.01-2 43.624.201.01-2 43.632.201.01-2	18 24 32

LIBRARY CODES

STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0082	LAB SCANBODY	DAS_C_E_0082
DYNAMIC µSCANBODY (LAB/CLIN)	DAS_I_10_0082 DAS_I_12_0082	DYNAMIC µSCANBODY (LAB/CLIN)	DAS_C_I_10_0082 DAS_C_I_12_0082




LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging



COMPATIBLE with 0083

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
1,2 mm				mm				mm				mm			
R	31.323.083.01-2	45°	25°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.313.083.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®		
GINGIVAL HEIGHT		
α_s	α_s	α_s
CH=5mm	CH=7mm	CH=9mm
R	-	-
NR	-	-

DYNAMIC µSCANBODY (LAB/CLIN)		DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
52.410.103.01-2	10	50.313.083.01-2	43.621.410.01-2	34.613.083.01-2
			43.624.410.01-2	
			43.630.410.01-2	
52.412.103.01-2	12			

DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.318.076.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

STRAIGHT SCREWS			
STRAIGHT SCREW	SCREWDRIVER	-	ANALOG LAB SCANBODY
40.318.012.02-2	-		30.413.002.01-2


LIBRARY CODES	
STANDARD LIBRARY	
LAB SCANBODY	DAS_E_0083
DYNAMIC µSCANBODY (LAB/CLIN)	DAS_I_10_0083
	DAS_I_12_0083

CAPTIVE SCREW LIBRARY	
STANDARD LIBRARY	
LAB SCANBODY	DAS_C_E_0083
DYNAMIC µSCANBODY (LAB/CLIN)	DAS_C_I_10_0083
	DAS_C_I_12_0083

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

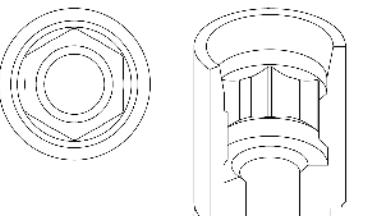

COMPATIBLE with 0084

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
1,2 mm				mm				mm				mm			
R	31.321.084.01-2	30°	-	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.311.084.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®		
GINGIVAL HEIGHT		
α_s	α_s	α_s
CH=5mm	CH=7mm	CH=9mm
R	-	-
NR	-	-

DYNAMIC µSCANBODY (LAB/CLIN)		DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
-	-	-	-	-
-	-	-	-	-
-	-	-	-	-

DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.314.076.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

STRAIGHT SCREWS			
STRAIGHT SCREW	SCREWDRIVER	Star 1.50	ANALOG LAB SCANBODY
40.314.003.03-2	-	43.601.103.02-2	30.410.006.01-2


LIBRARY CODES	
STANDARD LIBRARY	
LAB SCANBODY	DAS_E_0084
DYNAMIC µSCANBODY (LAB/CLIN)	-
	-

CAPTIVE SCREW LIBRARY	
STANDARD LIBRARY	
LAB SCANBODY	-
DYNAMIC µSCANBODY (LAB/CLIN)	-
	-

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

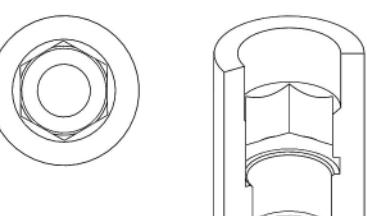

COMPATIBLE with 0085


STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
		mm				mm				mm				mm	
R	31.324.085.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.314.085.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®															
GINGIVAL HEIGHT			α_s	α_s	α_s	CH=5mm			CH=7mm			CH=9mm			
R	-			-			-			-			-		
NR	-			-			-			-			-		

DYNAMIC μ SCANBODY (LAB/CLIN)			DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL				
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	α_{dp}	DYNAMIC MILLING TOOL	SHANK	α_{di}
52.410.117.01-2	10			43.621.410.01-2			33.345.856.01-2	3	
		50.314.085.01-2		43.624.410.01-2			33.445.856.01-2	4	25°
52.412.117.01-2	12			43.630.410.01-2	34.614.085.01-2		33.645.856.01-2	6	

DYNAMIC SCREWS				
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	
41.316.081.01-2	-		43.618.201.01-2	18
			43.624.201.01-2	24
			43.632.201.01-2	32

STRAIGHT SCREWS				
STRAIGHT SCREW	SCREWDRIVER Hex. 1.25	ANALOG	LAB SCANBODY	
40.316.004.02-2	43.601.104.01-2	-	30.413.002.01-2	



LIBRARY CODES

STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0085	LAB SCANBODY	DAS_C_E_0085
DYNAMIC μ SCANBODY (LAB/CLIN)	DAS_L_10_0085	DYNAMIC μ SCANBODY (LAB/CLIN)	DAS_C_L_10_0085
	DAS_L_12_0085		DAS_C_L_12_0085

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

COMPATIBLE with 0086

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
		mm				mm				mm				mm	
R	31.325.086.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.315.086.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®															
GINGIVAL HEIGHT			α_s	α_s	α_s	CH=5mm			CH=7mm			CH=9mm			
R	-			-			-			-			-		
NR	-			-			-			-			-		

DYNAMIC μ SCANBODY (LAB/CLIN)			DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL				
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	α_{dp}	DYNAMIC MILLING TOOL	SHANK	α_{di}
41.316.081.01-2	-			43.618.201.01-2	18				
				43.624.201.01-2	24				
				43.632.201.01-2	32				

DYNAMIC SCREWS				
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	
41.316.081.01-2	-		43.618.201.01-2	18
			43.624.201.01-2	24
			43.632.201.01-2	32

STRAIGHT SCREWS				
STRAIGHT SCREW	SCREWDRIVER Hex. 1.25	ANALOG	LAB SCANBODY	
40.316.004.02-2	43.601.104.01-2	-	30.415.007.01-2	

LIBRARY CODES

STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0086	LAB SCANBODY	DAS_C_E_0086
DYNAMIC μ SCANBODY (LAB/CLIN)	-	DYNAMIC μ SCANBODY (LAB/CLIN)	-
		</	

COMPATIBLE with 0090

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
1 mm				mm				mm				mm			
R	31.321.090.01-2	45°	24°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.311.090.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®														
GINGIVAL HEIGHT			α_s	α_s	α_s	CH=5mm			CH=7mm			CH=9mm		
R	-			-			-			-				
NR	-			-			-			-				

DYNAMIC µSCANBODY (LAB/CLIN)		DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
-	-			
-	-			

COBALT-CHROME	α_{dp}

DYNAMIC MILLING TOOL	SHANK	α_{di}
33.325.472.01-2*	3	
33.425.472.01-2*	4	25°
33.625.472.01-2*	6	

DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.314.074.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

STRAIGHT SCREW	SCREWDRIVER Hex. 1.27
40.314.005.01-2	43.601.105.01-2

ANALOG	LAB SCANBODY
-	30.410.006.01-2

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0090	LAB SCANBODY	DAS_C_E_0090
DYNAMIC µSCANBODY (LAB/CLIN)	-	DYNAMIC µSCANBODY (LAB/CLIN)	-

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

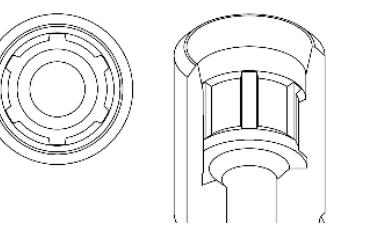

COMPATIBLE with 0091

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
1,2 mm				mm				mm				mm			
R	31.324.091.01-2	38°	18°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.314.091.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®															
GINGIVAL HEIGHT			α_s	α_s	α_s	CH=5mm			CH=7mm			CH=9mm			
R	-			-			-			-			-		
NR	-			-			-			-			-		

DYNAMIC µSCANBODY (LAB/CLIN)		DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
52.410.102.01-2	10		43.621.410.01-2	
			43.624.410.01-2	34.614.091.01-2
52.412.102.01-2	12		43.630.410.01-2	

DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.320.082.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

STRAIGHT SCREW	SCREWDRIVER Hex. 1.27
40.320.005.01-2	43.601.105.01-2

ANALOG	LAB SCANBODY
-	30.413.002.01-2

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0091	LAB SCANBODY	DAS_C_E_0091
DYNAMIC µSCANBODY (LAB/CLIN)	DAS_I_10_0091	DYNAMIC µSCANBODY (LAB/CLIN)	DAS_C_I_10_0091
	DAS_I_12_0091	DYNAMIC µSCANBODY (LAB/CLIN)	DAS_C_I_12_0091

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

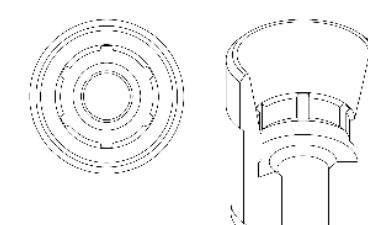

COMPATIBLE with 0092

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
1 mm		mm		mm		mm		mm		mm		mm		mm	
R	31.325.092.01-2	45°	25°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.315.092.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®			
GINGIVAL HEIGHT α_s α_s α_s			
CH=5mm CH=7mm CH=9mm			
R	-	-	-
NR	-	-	-

DYNAMIC µSCANBODY (LAB/CLIN)		DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
52.410.129.01-2	10	50.315.092.01-2	43.621.410.01-2	34.615.092.01-2
			43.624.410.01-2	
52.412.129.01-2	12		43.630.410.01-2	


COBALT-CHROME	α_{dp}
DYNAMIC MILLING TOOL	SHANK
33.390.958.01-2	3
33.490.958.01-2	4
33.690.958.01-2	6

DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.320.082.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

STRAIGHT SCREW	SCREWDRIVER Hex. 1.27
40.320.005.01-2	43.601.105.01-2
22.615.092.01-2	30.415.007.01-2

LIBRARY CODES			
STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0092	LAB SCANBODY	DAS_C_E_0092
DYNAMIC µSCANBODY (LAB/CLIN)	DAS_I_10_0092	DYNAMIC µSCANBODY (LAB/CLIN)	DAS_C_I_10_0092
	DAS_I_12_0092		DAS_C_I_12_0092

LIBRARY OPTIONS	
GH = Gingival Height	
CH = Cement Height	
α_s = Standard maximum angulation	
α_c = Captive maximum angulation	
α_{di} = Direct to implant maximum angulation	
α_{dp} = Dynamic Premilled maximum angulation	
R = Rotational / Non-Engaging	
NR = Non Rotational / Engaging	

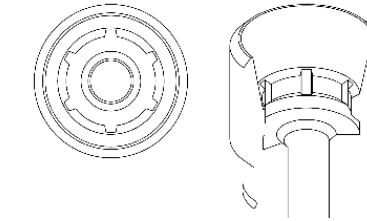

COMPATIBLE with 0096

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
0,6 mm		mm		mm		mm		mm		mm		mm		mm	
R	31.324.096.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.314.096.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®			
GINGIVAL HEIGHT α_s α_s α_s			
CH=5mm CH=7mm CH=9mm			
R	-	-	-
NR	-	-	-

DYNAMIC µSCANBODY (LAB/CLIN)		DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
52.410.110.01-2	10	50.314.096.01-2	43.621.410.01-2	34.614.096.01-2
			43.624.410.01-2	
52.412.110.01-2	12		43.630.410.01-2	


COBALT-CHROME	α_{dp}
DYNAMIC MILLING TOOL	SHANK
33.390.958.01-2	3
33.490.958.01-2	4
33.690.958.01-2	6

DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.320.067.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

STRAIGHT SCREW	SCREWDRIVER TORX T6
40.320.007.01-2	43.601.107.01-2
22.614.096.01-2	30.414.008.01-2

LIBRARY CODES			
STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0096	LAB SCANBODY	DAS_C_E_0096
DYNAMIC µSCANBODY (LAB/CLIN)	DAS_I_10_0096	DYNAMIC µSCANBODY (LAB/CLIN)	DAS_C_I_10_0096
	DAS_I_12_0096		DAS_C_I_12_0096

LIBRARY OPTIONS	
GH = Gingival Height	
CH = Cement Height	
α_s = Standard maximum angulation	
α_c = Captive maximum angulation	
α_{di} = Direct to implant maximum angulation	
α_{dp} = Dynamic Premilled maximum angulation	
R = Rotational / Non-Engaging	
NR = Non Rotational / Engaging	

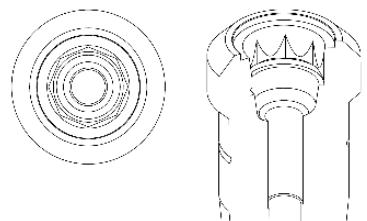

COMPATIBLE with 0101

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
		0,5 mm				mm				mm				mm	
R	31.323.101.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	-	-	-	-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®			
GINGIVAL HEIGHT α_s α_s α_s			
CH=5mm CH=7mm CH=9mm			
R	-	-	-
NR	-	-	-

DYNAMIC μ SCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL	SCANALOG	
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	DYNAMIC MILLING TOOL	SHANK	α_{dp} α_{di}
-	-	-	-	-	-	-	-	-
-	-	-	-	-	-	-	-	-
-	-	-	-	-	-	-	-	-
								23.413.101.01-2

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER TORX T6	ANALOG	LAB SCANBODY
41.314.043.01-2	-	43.618.201.01-2	18	40.314.007.01-2	43.601.107.01-2	-	30.413.005.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				


LIBRARY CODES	
STANDARD LIBRARY	
LAB SCANBODY	DAS_E_0101
DYNAMIC μ SCANBODY (LAB/CLIN)	-
SCANALOG	DAS_SA_0101

CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_C_E_0101
DYNAMIC μ SCANBODY (LAB/CLIN)	-
SCANALOG	DAS_C_SA_0101

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height

 α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

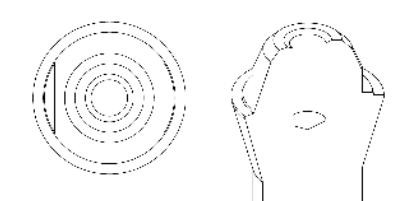

COMPATIBLE with 0102

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
		1,8 mm													
R	31.322.102.01-2	38°	18°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.312.102.01-2	-	-	-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®			
GINGIVAL HEIGHT α_s α_s α_s			
1,8 mm CH=5mm CH=7mm CH=9mm			
R	31.322.102.21-2	25°	15°
NR	31.312.102.21-2	-	-

DYNAMIC μ SCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL	SCANALOG	
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	DYNAMIC MILLING TOOL	SHANK	α_{dp}
-	-	-	-	-	-	-	-	-
-	-	-	-	-	-	-	-	-
-	-	-	-	-	-	-	-	-
								23.413.101.01-2

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER TORX T6	ANALOG	LAB SCANBODY
41.317.065.01-2	-	43.618.201.01-2	18	40.317.005.02-2	43.601.105.01-2	-	30.412.001.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				


LIBRARY CODES	
STANDARD LIBRARY	
LAB SCANBODY	DAS_E_0102
DYNAMIC μ SCANBODY (LAB/CLIN)	DAS_I_10_0102 DAS_IG_10_0102 DAS_I_12_0102 DAS_IG_12_0102
SCANALOG	DAS_SA_0102

CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_C_E_0102
DYNAMIC μ SCANBODY (LAB/CLIN)	DAS_C_I_10_0102 DAS_C_IG_10_0102 DAS_C_I_12_0102 DAS_C_IG_12_0102
SCANALOG	DAS_C_SA_0102

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height
IG = Adaptor (3mm)

 α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

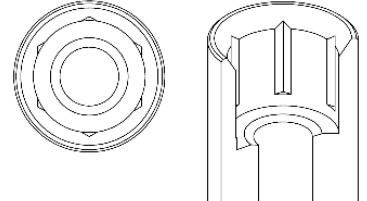

COMPATIBLE with 0109

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
		mm				mm				mm				mm	
R	31.322.109.01-2	45°	29°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.312.109.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®

GINGIVAL HEIGHT		
α_s	α_s	α_s
CH=5mm	CH=7mm	CH=9mm
R	-	-
NR	-	-

DYNAMIC μ SCANBODY (LAB/CLIN)

DIGITAL ANALOG		DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL					
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	α_{dp}	DYNAMIC MILLING TOOL	SHANK	α_{di}
52.410.128.01-2	10	50.312.109.01-2	43.621.415.01-2	34.612.109.01-2			33.360.754.01-2*	3	
52.412.128.01-2	12						33.460.754.01-2*	4	25°
							33.660.754.01-2*	6	

DYNAMIC SCREWS

DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.314.070.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0109	LAB SCANBODY	DAS_C_E_0109
DYNAMIC μ SCANBODY (LAB/CLIN)	DAS_L_10_0109	DYNAMIC μ SCANBODY (LAB/CLIN)	DAS_C_L_10_0109
	DAS_L_12_0109		DAS_C_L_12_0109

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

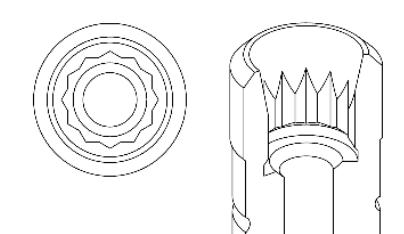

COMPATIBLE with 0110

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
		mm				mm				mm				mm	
R	31.320.110.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.310.110.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®

GINGIVAL HEIGHT		
α_s	α_s	α_s
CH=5mm	CH=7mm	CH=9mm
R	-	-
NR	-	-

DYNAMIC μ SCANBODY (LAB/CLIN)

DIGITAL ANALOG		DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL					
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	α_{dp}	DYNAMIC MILLING TOOL	SHANK	α_{di}
-	-	-	-	-	33.360.754.01-2*	3			
-	-	-	-	-	33.460.754.01-2*	4			
-	-	-	-	-	33.660.754.01-2*	6			

DYNAMIC SCREWS

DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.318.083.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0110	LAB SCANBODY	DAS_C_E_0110
DYNAMIC μ SCANBODY (LAB/CLIN)	-	DYNAMIC μ SCANBODY (LAB/CLIN)	-
	-		-

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

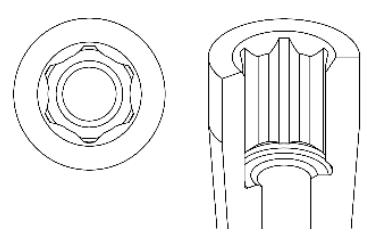

COMPATIBLE with 0111

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
		0,4 mm				mm				mm				mm	
R	31.323.111.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.313.111.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®		
GINGIVAL HEIGHT		
	α_s	α_s
	CH=5mm	CH= 7mm
	CH= 9mm	
R	-	
NR	-	


DYNAMIC μ SCANBODY (LAB/CLIN)		DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
-	-			
-	-			

COBALT-CHROME	α_{dp}	DYNAMIC MILLING TOOL	SHANK	α_{di}

DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.318.083.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

STRAIGHT SCREW	SCREWDRIVER TORX T6	ANALOG	LAB SCANBODY
40.318.007.01-2	43.601.107.01-2	-	30.413.002.01-2

LIBRARY CODES	
STANDARD LIBRARY	
LAB SCANBODY	DAS_E_0111
DYNAMIC μ SCANBODY (LAB/CLIN)	-
LAB SCANBODY	DAS_C_E_0111
DYNAMIC μ SCANBODY (LAB/CLIN)	-

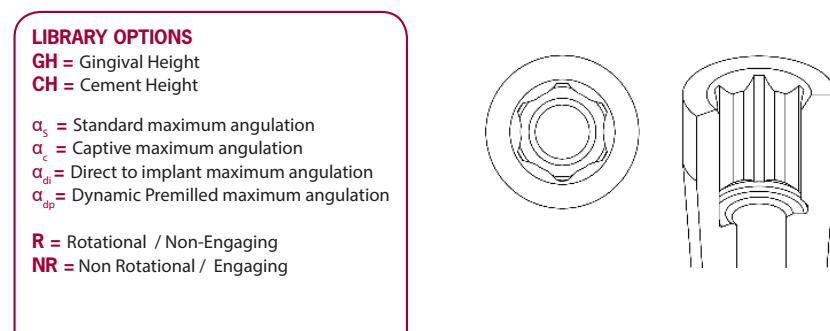

COMPATIBLE with 0120

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
		1 mm				mm				mm				mm	
R	31.323.121.01-2	45°	25°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.313.121.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®		
GINGIVAL HEIGHT		
	α_s	α_s
	CH=5mm	CH= 7mm
	CH= 9mm	
R	-	
NR	-	

DYNAMIC μ SCANBODY (LAB/CLIN)		DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
-	-			
-	-			

COBALT-CHROME	α_{dp}	DYNAMIC MILLING TOOL	SHANK	α_{di}

DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.316.080.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

STRAIGHT SCREW	SCREWDRIVER TORX T6	ANALOG	LAB SCANBODY
40.316.005.07-2	43.601.105.01-2	-	30.413.002.01-2


LIBRARY CODES	
STANDARD LIBRARY	
LAB SCANBODY	DAS_E_0120
DYNAMIC μ SCANBODY (LAB/CLIN)	-
LAB SCANBODY	DAS_C_E_0120
DYNAMIC μ SCANBODY (LAB/CLIN)	-

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

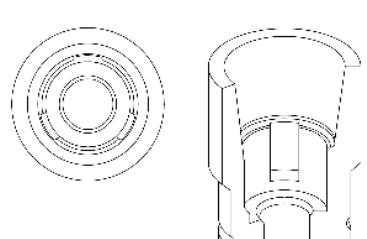

COMPATIBLE with 0121

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
1 mm		mm		mm		mm		mm		mm		mm		mm	
R	31.323.121.01-2	45°	25°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.313.121.01-2	-	-	-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®		
GINGIVAL HEIGHT		
α_s	α_s	α_s
CH=5mm	CH=7mm	CH=9mm
R	-	-
NR	-	-

DYNAMIC µSCANBODY (LAB/CLIN)		DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
-	-	-	-	-
-	-	-	-	-
-	-	-	-	-

COBALT-CHROME	α_{dp}
-	-
-	-


DYNAMIC MILLING TOOL	SHANK	α_{di}
33.360.754.01-2	3	20°
33.460.754.01-2	4	
33.660.754.01-2	6	

DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.316.080.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

STRAIGHT SCREW	SCREWDRIVER Hex. 1.27	ANALOG	LAB SCANBODY
40.316.005.07-2	43.601.105.01-2	-	30.413.002.01-2

LIBRARY CODES			
STANDARD LIBRARY	CAPTIVE SCREW LIBRARY	STRAIGHT SCREW	SCREWDRIVER UNIGRIP
LAB SCANBODY	DAS_E_0121	LAB SCANBODY	DAS_C_E_0121
DYNAMIC µSCANBODY (LAB/CLIN)	-	DYNAMIC µSCANBODY (LAB/CLIN)	-

LIBRARY OPTIONS			
GH = Gingival Height	CH = Cement Height	α _s = Standard maximum angulation	α _c = Captive maximum angulation
		α _{di} = Direct to implant maximum angulation	α _{dp} = Dynamic Premilled maximum angulation
		R = Rotational / Non-Engaging	NR = Non Rotational / Engaging



COMPATIBLE with 0124

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
1,4 mm		mm		mm		mm		mm		mm		mm		mm	
R	31.324.124.01-2	42°	19°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.314.124.01-2	-	-	-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®		
GINGIVAL HEIGHT		
α_s	α_s	α_s
CH=5mm	CH=7mm	CH=9mm
R	-	-
NR	-	-

DYNAMIC µSCANBODY (LAB/CLIN)		DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
-	-	-	-	-
-	-	-	-	-
-	-	-	-	-

COBALT-CHROME	α_{dp}
-	-
-	-


DYNAMIC MILLING TOOL	SHANK	α_{di}
33.335.758.01-2	3	30°
33.435.758.01-2	4	
33.635.758.01-2	6	

DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.320.075.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

STRAIGHT SCREW	SCREWDRIVER Hex. 1.27	ANALOG	LAB SCANBODY
40.320.008.02-2	43.601.108.01-2	-	30.414.003.01-2

LIBRARY CODES			
STANDARD LIBRARY	CAPTIVE SCREW LIBRARY	STRAIGHT SCREW	SCREWDRIVER UNIGRIP
LAB SCANBODY	DAS_E_0124	LAB SCANBODY	DAS_C_E_0124
DYNAMIC µSCANBODY (LAB/CLIN)	-	DYNAMIC µSCANBODY (LAB/CLIN)	-

LIBRARY OPTIONS			
GH = Gingival Height	CH = Cement Height	α _s = Standard maximum angulation	α _c = Captive maximum angulation
		α _{di} = Direct to implant maximum angulation	α _{dp} = Dynamic Premilled maximum angulation
		R = Rotational / Non-Engaging	NR = Non Rotational / Engaging

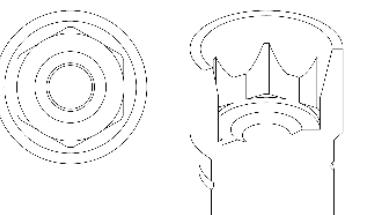

COMPATIBLE with 0125

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
1,1 mm				mm				mm				mm			
R	31.323.125.01-2	42°	20°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.313.125.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®		
GINGIVAL HEIGHT		
α_s	α_s	α_s
CH=5mm	CH=7mm	CH=9mm
R	-	-
NR	-	-

DYNAMIC µSCANBODY (LAB/CLIN)		DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
52.410.117.01-2	10	50.313.125.01-2	43.621.410.01-2	34.613.125.01-2
			43.624.410.01-2	
			43.630.410.01-2	
52.412.117.01-2	12			

DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.316.078.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

STRAIGHT SCREWS			
STRAIGHT SCREW	SCREWDRIVER TORX T6	ANALOG	LAB SCANBODY
40.316.007.01-2	43.601.107.01-2	-	30.413.002.01-2


LIBRARY CODES	
STANDARD LIBRARY	
LAB SCANBODY	DAS_E_0125
DYNAMIC µSCANBODY (LAB/CLIN)	DAS_I_10_0125
	DAS_I_12_0125

CAPTIVE SCREW LIBRARY	
STANDARD LIBRARY	
LAB SCANBODY	DAS_C_E_0125
DYNAMIC µSCANBODY (LAB/CLIN)	DAS_C_I_10_0125
	DAS_C_I_12_0125

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

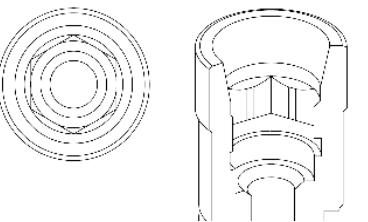

COMPATIBLE with 0128

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
2,5 mm															
R	31.322.128.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	-			-	-	-	-	-	-	-	-	-	-	-	-


DYNAMIC 3TIBASE®		
GINGIVAL HEIGHT		
α_s	α_s	α_s
CH=5mm	CH=7mm	CH=9mm
-	-	-
-	-	-

DYNAMIC µSCANBODY (LAB/CLIN)		DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
41.320.044.01-2	-	-	43.618.201.01-2	18
			43.624.201.01-2	24
			43.632.201.01-2	32

DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
40.320.003.05-2	-	43.601.103.01-2	-
		-	30.413.002.01-2

LIBRARY CODES	
STANDARD LIBRARY	
LAB SCANBODY	DAS_E_0128
DYNAMIC µSCANBODY (LAB/CLIN)	-
	-

CAPTIVE SCREW LIBRARY	
STANDARD LIBRARY	
LAB SCANBODY	DAS_C_E_0128
DYNAMIC µSCANBODY (LAB/CLIN)	-
	-

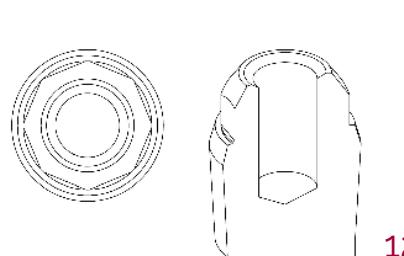

COMPATIBLE with 0129

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
		mm				mm				mm				mm	
R	-			-		-		-		-		-		-	
NR	-			-		-		-		-		-		-	

DYNAMIC 3TIBASE®		
GINGIVAL HEIGHT		
α_s	α_s	α_s
CH=5mm	CH=7mm	CH=9mm
R	-	
NR	-	

DYNAMIC µSCANBODY (LAB/CLIN)		DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
52.410.130.01-2	10		43.621.410.01-2	
		50.315.129.01-2	43.624.410.01-2	34.615.129.01-2
			43.630.410.01-2	
52.412.130.01-2	12			


COBALT-CHROME	α_{dp}
DYNAMIC MILLING TOOL	SHANK
33.390.958.01-2	3
33.490.958.01-2	4
33.690.958.01-2	6

DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.320.090.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

STRAIGHT SCREW	SCREWDRIVER UNIGRIP
40.320.008.03-2	43.601.108.01-2
22.615.129.01-2	30.415.007.01-2

LIBRARY CODES	
STANDARD LIBRARY	CAPTIVE SCREW LIBRARY
LAB SCANBODY	LAB SCANBODY

LIBRARY OPTIONS	
GH = Gingival Height	
CH = Cement Height	
α_s = Standard maximum angulation	
α_c = Captive maximum angulation	
α_{di} = Direct to implant maximum angulation	
α_{dp} = Dynamic Premilled maximum angulation	
R = Rotational / Non-Engaging	
NR = Non Rotational / Engaging	



COMPATIBLE with 0130

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
		mm								mm				mm	
R	31.322.130.01-2	38°	29°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.312.130.01-2			-	-	-	-	-	-	-	-	-	-	-	-


DYNAMIC 3TIBASE®		
GINGIVAL HEIGHT		
α_s	α_s	α_s
CH=5mm	CH=7mm	CH=9mm
R	-	
NR	-	

DYNAMIC µSCANBODY (LAB/CLIN)		DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
41.316.081.01-2			43.618.201.01-2	18
			43.624.201.01-2	24
			43.632.201.01-2	32

DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
40.316.005.08-2		43.601.105.01-2	
		-	30.412.001.01-2

LIBRARY CODES	
STANDARD LIBRARY	CAPTIVE SCREW LIBRARY
LAB SCANBODY	LAB SCANBODY

LIBRARY OPTIONS	
GH = Gingival Height	
CH = Cement Height	
α_s = Standard maximum angulation	
α_c = Captive maximum angulation	
α_{di} = Direct to implant maximum angulation	
α_{dp} = Dynamic Premilled maximum angulation	
R = Rotational / Non-Engaging	
NR = Non Rotational / Engaging	

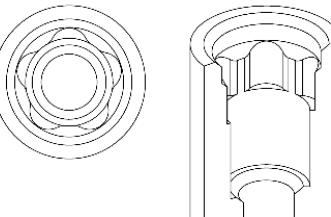

COMPATIBLE with 0131

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
0,5 mm				mm				mm				mm			
R	31.323.131.01-2	45°	29°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.313.131.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®

GINGIVAL HEIGHT		
α_s	α_s	α_s
CH=5mm	CH=7mm	CH=9mm
R	-	-
NR	-	-

DYNAMIC µSCANBODY (LAB/CLIN)

SCANBODY		HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
-	-		-	-	-
-	-		-	-	-

DIGITAL ANALOG

DYNAMIC PRE-MILLED

COBALT-CHROME		α_{dp}
DYNAMIC MILLING TOOL	SHANK	α_{di}
33.345.804.01-2	3	
33.445.804.01-2	4	20°
33.645.804.01-2	6	

DYNAMIC SCREWS

DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.316.081.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

STRAIGHT SCREWS

STRAIGHT SCREW	SCREWDRIVER Hex. 1.27	ANALOG	LAB SCANBODY
40.316.005.08-2	43.601.105.01-2	-	30.413.002.01-2
		-	

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0131	LAB SCANBODY	DAS_C_E_0131
DYNAMIC µSCANBODY (LAB/CLIN)	-	DYNAMIC µSCANBODY (LAB/CLIN)	-

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

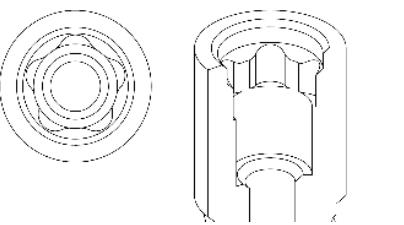

COMPATIBLE with 0132

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
0,5 mm				mm				mm				mm			
R	31.324.132.01-2	45°	28°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.314.132.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®

GINGIVAL HEIGHT		
α_s	α_s	α_s
CH=5mm	CH=7mm	CH=9mm
R	-	-
NR	-	-

DYNAMIC µSCANBODY (LAB/CLIN)

SCANBODY		HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
-	-		-	-	-
-	-		-	-	-
-	-		-	-	-

DIGITAL ANALOG

DYNAMIC PRE-MILLED

COBALT-CHROME		α_{dp}
DYNAMIC MILLING TOOL	SHANK	α_{di}
33.345.856.01-2	3	
33.445.856.01-2	4	25°
33.645.856.01-2	6	

DYNAMIC SCREWS

DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.316.081.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

STRAIGHT SCREWS

STRAIGHT SCREW	SCREWDRIVER Hex. 1.27	ANALOG	LAB SCANBODY
40.316.005.08-2	43.601.105.01-2	-	30.414.003.01-2
		-	

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0132	LAB SCANBODY	DAS_C_E_0132
DYNAMIC µSCANBODY (LAB/CLIN)	-	DYNAMIC µSCANBODY (LAB/CLIN)	-

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

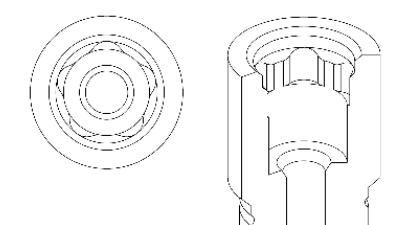

COMPATIBLE with 0135

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
1 mm				mm				mm				mm			
R	31.320.135.01-2	45°	-	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.310.135.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®		
GINGIVAL HEIGHT		
α_s	α_s	α_s
CH=5mm	CH=7mm	CH=9mm
R	-	-
NR	-	-

DYNAMIC µSCANBODY (LAB/CLIN)		DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
-	-	-	-	-
-	-	-	-	-

DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.314.080.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32



STRAIGHT SCREWS			
STRAIGHT SCREW	SCREWDRIVER TORX T6	ANALOG	LAB SCANBODY
40.314.007.02-2	43.601.107.01-2	-	30.410.006.01-2

LIBRARY CODES	
STANDARD LIBRARY	
LAB SCANBODY	DAS_E_0135
DYNAMIC µSCANBODY (LAB/CLIN)	-
CAPTIVE SCREW LIBRARY	
LAB SCANBODY	-
DYNAMIC µSCANBODY (LAB/CLIN)	-

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

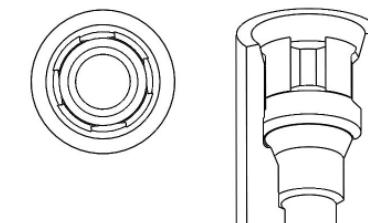


LIBRARY CODES	
STANDARD LIBRARY	
LAB SCANBODY	DAS_E_0136
DYNAMIC µSCANBODY (LAB/CLIN)	DAS_I_10_0136
CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_C_E_0136
DYNAMIC µSCANBODY (LAB/CLIN)	DAS_C_I_10_0136
	DAS_I_12_0136

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

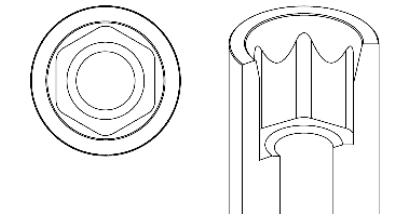

COMPATIBLE with 0137


STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
		mm				mm				mm				mm	
R	31.324.137.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.314.137.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®			
GINGIVAL HEIGHT	α_s	α_s	α_s
CH=5mm	CH=7mm	CH=9mm	
-	-	-	-
-	-	-	-

DYNAMIC µSCANBODY (LAB/CLIN)		DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
-	-			
-	-			

DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.320.044.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

STRAIGHT SCREWS			
STRAIGHT SCREW	SCREWDRIVER TORX T6	ANALOG	LAB SCANBODY
40.320.007.04-2	43.601.107.01-2	-	30.414.008.01-2

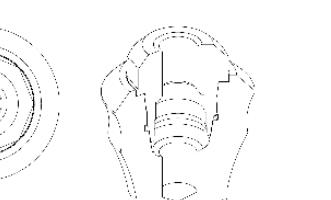

LIBRARY CODES

STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0137	LAB SCANBODY	DAS_C_E_0137
DYNAMIC µSCANBODY (LAB/CLIN)	-	DYNAMIC µSCANBODY (LAB/CLIN)	-
			-

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

COMPATIBLE with 0149

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
		mm				mm				mm				mm	
R	31.323.149.01-2	45°	29°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.313.149.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®			
GINGIVAL HEIGHT	α_s	α_s	α_s
CH=5mm	CH=7mm	CH=9mm	
-	-	-	-
-	-	-	-

DYNAMIC µSCANBODY (LAB/CLIN)		DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
52.410.132.01-2	10		43.621.410.01-2	
			43.624.410.01-2	
			43.630.410.01-2	
50.310.161.01-2				
52.412.132.01-2	12			

* Only for R

DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.316.079.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

STRAIGHT SCREWS			
STRAIGHT SCREW	SCREWDRIVER TORX T6	ANALOG	LAB SCANBODY
40.316.014.01-2	30.413.002.01-2	-	

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0149	LAB SCANBODY	DAS_C_E_0149
DYNAMIC µSCANBODY (LAB/CLIN)	-	DYNAMIC µSCANBODY (LAB/CLIN)	-
		-	-

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

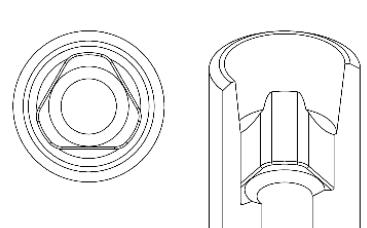

COMPATIBLE with 0150

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
		mm				mm				mm				mm	
R	31.323.150.01-2	45°	-	-	-	-	-	-	-	-	-	-	-	-	-
NR	-	-	-	-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®			
GINGIVAL HEIGHT	α_s	α_s	α_s
CH=5mm	α_s	α_s	α_s
CH= 7mm	-	-	-
CH= 9mm	-	-	-


DYNAMIC μ SCANBODY (LAB/CLIN)	DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL	
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
-	-	-	-	-
-	-	-	-	-
-	-	-	-	-

DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.314.046.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

STRAIGHT SCREWS			
STRAIGHT SCREW	SCREWDRIVER Hex. 1.25	ANALOG	LAB SCANBODY
40.314.004.04-2	43.601.104.01-2	-	30.413.005.01-2

LIBRARY CODES	
STANDARD LIBRARY	
LAB SCANBODY	DAS_E_0150
DYNAMIC μ SCANBODY (LAB/CLIN)	-
LAB SCANBODY	-
DYNAMIC μ SCANBODY (LAB/CLIN)	-
LAB SCANBODY	-
DYNAMIC μ SCANBODY (LAB/CLIN)	-

LIBRARY OPTIONS	
GH = Gingival Height	
CH = Cement Height	
α_s = Standard maximum angulation	
α_c = Captive maximum angulation	
α_{di} = Direct to implant maximum angulation	
α_{dp} = Dynamic Premilled maximum angulation	
R = Rotational / Non-Engaging	
NR = Non Rotational / Engaging	

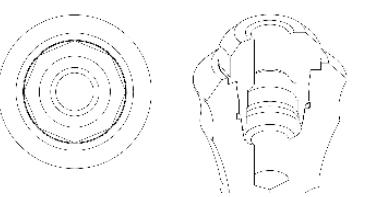

COMPATIBLE with 0151

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
		mm				mm				mm				mm	
R	31.323.151.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
-	-	-	-	-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®			
GINGIVAL HEIGHT	α_s	α_s	α_s
CH=5mm	α_s	α_s	α_s
CH= 7mm	-	-	-
CH= 9mm	-	-	-


DYNAMIC μ SCANBODY (LAB/CLIN)	DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL	
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
52.409.123.01-2	9	50.313.151.01-2	43.621.410.01-2 43.624.410.01-2 43.630.410.01-2	34.613.151.01-2
-	-	-	-	-
-	-	-	-	-
-	-	-	-	-

DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.314.039.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

STRAIGHT SCREWS			
STRAIGHT SCREW	SCREWDRIVER Hex. 1.25	ANALOG	LAB SCANBODY
40.314.004.04-2	43.601.104.01-2	-	30.413.005.01-2

LIBRARY CODES	
STANDARD LIBRARY	
LAB SCANBODY	DAS_E_0151
DYNAMIC μ SCANBODY (LAB/CLIN)	DAS_I_9_0151
LAB SCANBODY	DAS_C_E_0151
DYNAMIC μ SCANBODY (LAB/CLIN)	DAS_C_I_9_0151

LIBRARY OPTIONS	
GH = Gingival Height	
CH = Cement Height	
α_s = Standard maximum angulation	
α_c = Captive maximum angulation	
α_{di} = Direct to implant maximum angulation	
α_{dp} = Dynamic Premilled maximum angulation	
R = Rotational / Non-Engaging	
NR = Non Rotational / Engaging	

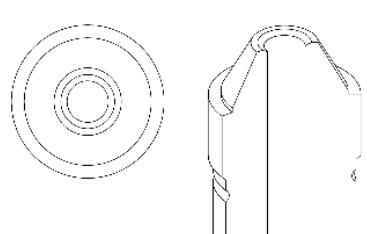

COMPATIBLE with 0152

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
1 mm				mm				mm				mm			
R	31.320.152.01-2	45°	-	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.310.152.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®			
GINGIVAL HEIGHT	α_s	α_s	α_s
CH=5mm	α_s	α_s	α_s
CH=7mm			
CH=9mm			

DYNAMIC μ SCANBODY (LAB/CLIN)		DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
-	-			
-	-			

DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.318.077.02-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

STRAIGHT SCREWS		
STRAIGHT SCREW	SCREWDRIVER	
ANALOG	-	
		30.410.006.01-2


LIBRARY CODES	
STANDARD LIBRARY	
LAB SCANBODY	DAS_E_0152
DYNAMIC μ SCANBODY (LAB/CLIN)	-
	-

CAPTIVE SCREW LIBRARY	
LAB SCANBODY	-
DYNAMIC μ SCANBODY (LAB/CLIN)	-
	-

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

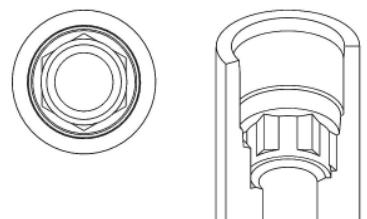

COMPATIBLE with 0159

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
1,5 mm				mm				mm				mm			
R	31.320.159.01-2	41°	17°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.310.159.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®			
GINGIVAL HEIGHT	α_s	α_s	α_s
CH=5mm	α_s	α_s	α_s
CH=7mm			
CH=9mm			

DYNAMIC μ SCANBODY (LAB/CLIN)		DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
52.410.128.01-2	10			
		50.310.159.01-2	43.621.415.01-2	34.610.159.01-2
		-	-	-

DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.314.067.02-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

STRAIGHT SCREWS		
STRAIGHT SCREW	SCREWDRIVER	
ANALOG	-	
		30.410.006.01-2


LIBRARY CODES	
STANDARD LIBRARY	
LAB SCANBODY	DAS_E_0159
DYNAMIC μ SCANBODY (LAB/CLIN)	-
	-

CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_C_E_0159
DYNAMIC μ SCANBODY (LAB/CLIN)	-
	-

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

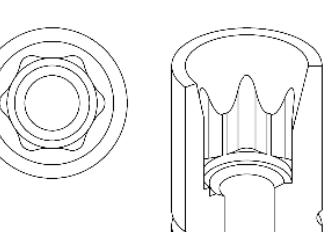

COMPATIBLE with 0160

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
		0,5 mm				mm				mm				mm	
R	31.320.160.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.310.160.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®		
GINGIVAL HEIGHT		
α_s	α_s	α_s
CH=5mm	CH=7mm	CH=9mm
-	-	-
-	-	-

DYNAMIC µSCANBODY (LAB/CLIN)		DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
52.410.131.01-2	10			
		50.310.160.01-2	43.621.415.01-2	34.610.160.01-2
52.412.131.01-2	12			

DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.316.078.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32


STRAIGHT SCREWS			
STRAIGHT SCREW	SCREWDRIVER TORX T6	ANALOG	LAB SCANBODY
40.316.007.01-2	43.601.107.01-2	22.610.160.01-2	30.410.006.01-2

LIBRARY CODES	
STANDARD LIBRARY	
LAB SCANBODY	DAS_E_0160
DYNAMIC µSCANBODY (LAB/CLIN)	DAS_I_10_0160
	DAS_I_12_0160
CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_C_E_0160
DYNAMIC µSCANBODY (LAB/CLIN)	DAS_C_I_10_0160
	DAS_C_I_12_0160

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

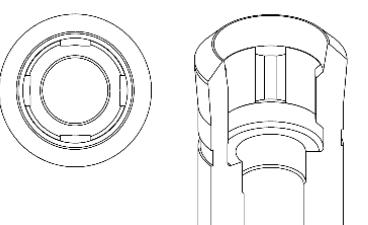

COMPATIBLE with 0161

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
		1,5 mm				mm				mm				mm	
R	31.320.161.01-2	45°	25°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.310.161.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®		
GINGIVAL HEIGHT		
α_s	α_s	α_s
CH=5mm	CH=7mm	CH=9mm
-	-	-
-	-	-

DYNAMIC µSCANBODY (LAB/CLIN)		DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
52.410.132.01-2	10			
		50.310.161.01-2	43.621.415.01-2	34.610.161.01-2
52.412.132.01-2	12			

DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.316.079.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32


STRAIGHT SCREWS			
STRAIGHT SCREW	SCREWDRIVER TORX T6	ANALOG	LAB SCANBODY
40.316.014.01-2	-	-	30.410.006.01-2

LIBRARY CODES	
STANDARD LIBRARY	
LAB SCANBODY	DAS_E_0161
DYNAMIC µSCANBODY (LAB/CLIN)	DAS_I_10_0161
	DAS_I_12_0161
CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_C_E_0161
DYNAMIC µSCANBODY (LAB/CLIN)	DAS_C_I_10_0161
	DAS_C_I_12_0161

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

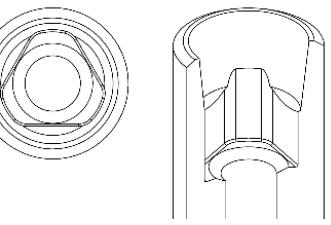

COMPATIBLE with 0162

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
1,5 mm				mm				mm				mm			
R	31.324.162.01-2	45°	24°	-	-	-	-	-	-	-	-	-	-	-	-
NR	-			-	-	-	-	-	-	-	-	-	-	-	-


DYNAMIC 3TIBASE®			
GINGIVAL HEIGHT	α_s	α_s	α_s
CH=5mm	α_s	α_s	α_s
CH= 7mm			
CH= 9mm			

DYNAMIC μ SCANBODY (LAB/CLIN)		DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
52.410.132.01-2	10	50.310.161.01-2	43.621.415.01-2	34.610.161.01-2
52.412.132.01-2	12			

* Only for R

DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.316.079.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

STRAIGHT SCREWS	
STRAIGHT SCREW	SCREWDRIVER
ANALOG	LAB SCANBODY
40.316.014.01-2	-

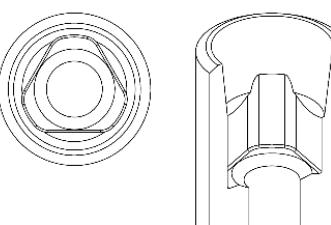

LIBRARY CODES

STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0162	LAB SCANBODY	DAS_C_E_0162
DYNAMIC μ SCANBODY (LAB/CLIN)	DAS_L_10_0162	DYNAMIC μ SCANBODY (LAB/CLIN)	DAS_C_L_10_0162
	DAS_L_12_0162		DAS_C_L_12_0162

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

COMPATIBLE with 0163

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
0,5 mm				mm				mm				mm			
R	31.323.163.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	-			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®			
GINGIVAL HEIGHT	α_s	α_s	α_s
CH=5mm	α_s	α_s	α_s
CH= 7mm			
CH= 9mm			

DYNAMIC μ SCANBODY (LAB/CLIN)		DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
52.408.112.01-2	8	50.313.163.01-2	43.620.411.01-2	34.613.163.01-2

DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.314.039.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

STRAIGHT SCREWS	
STRAIGHT SCREW	SCREWDRIVER
ANALOG	LAB SCANBODY
40.314.014.01-2	-

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0163	LAB SCANBODY	DAS_C_E_0163
DYNAMIC μ SCANBODY (LAB/CLIN)	DAS_I_10_0163	DYNAMIC μ SCANBODY (LAB/CLIN)	DAS_C_I_10_0163
	DAS_I_12_0163		DAS_C_I_12_0163

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

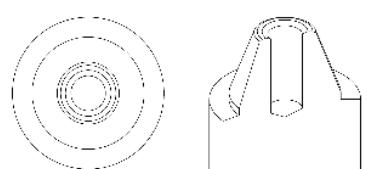

COMPATIBLE with 0164

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
1 mm		mm		mm		mm		mm		mm		mm		mm	
R	31.320.164.01-2	45°	21°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.310.164.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®		
GINGIVAL HEIGHT		
α_s	α_s	α_s
CH=5mm	CH=7mm	CH=9mm
-	-	-
-	-	-

DYNAMIC μ SCANBODY (LAB/CLIN)		DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
-	-			
-	-			


* Only for R

COBALT-CHROME	α_{dp}

DYNAMIC MILLING TOOL	SHANK	α_{di}
33.345.804.01-2*	3	
33.445.804.01-2*	4	25°
33.645.804.01-2*	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER	-
41.312.078.01-2	-	43.618.201.01-2	18			
		43.624.201.01-2	24			
		43.632.201.01-2	32			

ANALOG LAB SCANBODY

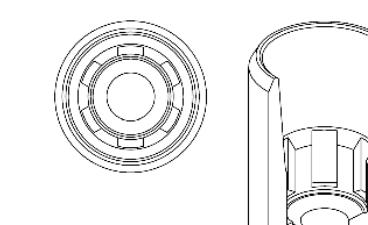

LIBRARY CODES

STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0164	LAB SCANBODY	DAS_C_E_0164
DYNAMIC μ SCANBODY (LAB/CLIN)	-	DYNAMIC μ SCANBODY (LAB/CLIN)	-

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

COMPATIBLE with 0165

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
1 mm		mm		mm		mm		mm		mm		mm		mm	
R	31.323.165.01-2	45°	25°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.313.165.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®		
GINGIVAL HEIGHT		
α_s	α_s	α_s
CH=5mm	CH=7mm	CH=9mm
-	-	-
-	-	-

DYNAMIC μ SCANBODY (LAB/CLIN)		DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
52.410.132.01-2	10		43.621.410.01-2	
		50.313.165.01-2	43.624.410.01-2	34.613.165.01-2
52.412.132.01-2	12		43.630.410.01-2	


* Only for R

COBALT-CHROME	α_{dp}

DYNAMIC MILLING TOOL	SHANK	α_{di}
33.345.804.01-2*	3	
33.445.804.01-2*	4	30°
33.645.804.01-2*	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER	-
41.314.076.01-2	-	43.618.201.01-2	18			
		43.624.201.01-2	24			
		43.632.201.01-2	32			

ANALOG LAB SCANBODY

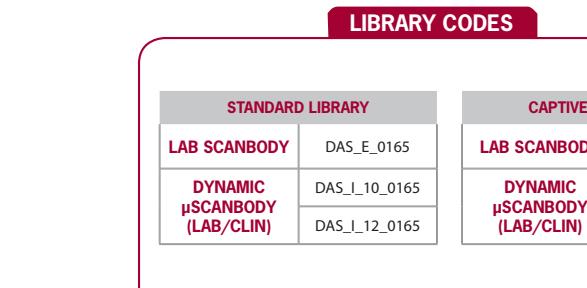

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0165	LAB SCANBODY	DAS_C_E_0165
DYNAMIC μ SCANBODY (LAB/CLIN)	-	DYNAMIC μ SCANBODY (LAB/CLIN)	-

LIBRARY OPTIONS

GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

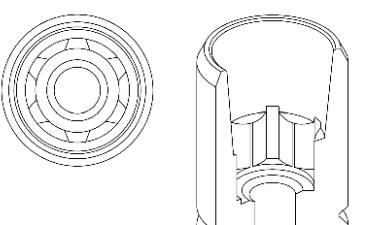

COMPATIBLE with 0166

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
		mm				mm				mm				mm	
R	31.320.166.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.310.166.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®		
GINGIVAL HEIGHT		
α_s	α_s	α_s
CH=5mm	CH=7mm	CH=9mm
-	-	-
-	-	-

DYNAMIC µSCANBODY (LAB/CLIN)		DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
-	-			
		-	-	-
-	-			


COBALT-CHROME	α_{dp}	DYNAMIC MILLING TOOL	SHANK	α_{di}
-	-	-	-	-
-	-	-	-	-
-	-	-	-	-

DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.314.084.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

STRAIGHT SCREW	SCREWDRIVER Hex. 1.25	ANALOG	LAB SCANBODY
40.314.004.02-2	43.601.104.01-2	-	30.410.006.01-2

LIBRARY CODES	
STANDARD LIBRARY	
LAB SCANBODY	DAS_E_0166
DYNAMIC µSCANBODY (LAB/CLIN)	-
CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_C_E_0166
DYNAMIC µSCANBODY (LAB/CLIN)	-

LIBRARY OPTIONS	
GH = Gingival Height	
CH = Cement Height	
α_s = Standard maximum angulation	
α_c = Captive maximum angulation	
α_{di} = Direct to implant maximum angulation	
α_{dp} = Dynamic Premilled maximum angulation	
R = Rotational / Non-Engaging	
NR = Non Rotational / Engaging	

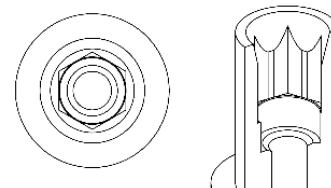

COMPATIBLE with 0167

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
		mm				mm				mm				mm	
R	31.322.167.01-2	43°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.312.167.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®		
GINGIVAL HEIGHT		
α_s	α_s	α_s
CH=5mm	CH=7mm	CH=9mm
-	-	-
-	-	-


DYNAMIC µSCANBODY (LAB/CLIN)		DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
52.410.117.01-2	10			
		50.313.167.03-2 (IG=3mm)	43.620.411.01-2 43.621.410.01-2 43.624.410.01-2 43.630.410.01-2	34.613.167.01-2
52.412.117.01-2	12			

DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.316.084.02-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

STRAIGHT SCREW	SCREWDRIVER Hex. 1.25	ANALOG	LAB SCANBODY
-	-	-	30.412.001.01-2

LIBRARY CODES	
STANDARD LIBRARY	
LAB SCANBODY	DAS_E_0167
DYNAMIC µSCANBODY (LAB/CLIN)	-
CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_C_E_0167
DYNAMIC µSCANBODY (LAB/CLIN)	-

LIBRARY OPTIONS	
GH = Gingival Height	
CH = Cement Height	
IG = Adaptor 3mm	
α_s = Standard maximum angulation	
α_c = Captive maximum angulation	
α_{di} = Direct to implant maximum angulation	
α_{dp} = Dynamic Premilled maximum angulation	
R = Rotational / Non-Engaging	
NR = Non Rotational / Engaging	

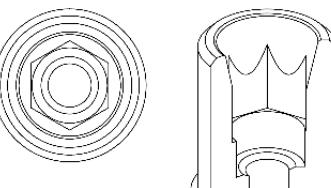

COMPATIBLE with 0168

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
		mm				mm				mm				mm	
R	31.323.168.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	-			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®			
GINGIVAL HEIGHT	α_s	α_s	α_s
CH=5mm	CH= 7mm	CH= 9mm	
-	-	-	-
-	-	-	-

DYNAMIC µSCANBODY (LAB/CLIN)		DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
-	-			
		-	-	-
-	-			

COBALT-CHROME	α_{dp}	DYNAMIC MILLING TOOL	SHANK	α_{di}
-	-	-	-	-
-	-	-	-	-
-	-	-	-	-

DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.314.039.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

STRAIGHT SCREW	SCREWDRIVER Hex. 1.27	ANALOG	LAB SCANBODY
40.314.004.03-2	43.601.104.01-2	-	30.413.005.01-2


LIBRARY CODES	
STANDARD LIBRARY	
LAB SCANBODY	DAS_E_0168
DYNAMIC µSCANBODY (LAB/CLIN)	-
DAS_E_0169	-

CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_C_E_0168
DYNAMIC µSCANBODY (LAB/CLIN)	-
DAS_C_E_0169	-

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

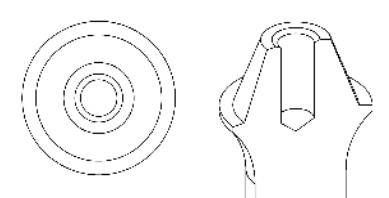

COMPATIBLE with 0169

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
		mm				mm				mm				mm	
R	31.322.169.01-2	45°	29°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.312.169.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®			
GINGIVAL HEIGHT	α_s	α_s	α_s
CH=5mm	CH= 7mm	CH= 9mm	
-	-	-	-
-	-	-	-

DYNAMIC µSCANBODY (LAB/CLIN)		DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
52.410.117.01-2	10		43.621.410.01-2	
		50.312.169.01-2	43.624.410.01-2	34.612.169.01-2
52.412.117.01-2	12		43.630.410.01-2	

COBALT-CHROME	α_{dp}	DYNAMIC MILLING TOOL	SHANK	α_{di}
-	-	-	-	-
-	-	-	-	-
-	-	-	-	-

DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.317.070.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

STRAIGHT SCREW	SCREWDRIVER Hex. 1.27	ANALOG	LAB SCANBODY
40.314.004.03-2	43.601.104.01-2	-	30.412.001.01-2


LIBRARY CODES	
STANDARD LIBRARY	
LAB SCANBODY	DAS_E_0169
DYNAMIC µSCANBODY (LAB/CLIN)	DAS_I_10_0169
DAS_E_0169	DAS_I_12_0169

CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_C_E_0169
DYNAMIC µSCANBODY (LAB/CLIN)	DAS_C_I_10_0169
DAS_C_E_0169	DAS_C_I_12_0169

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

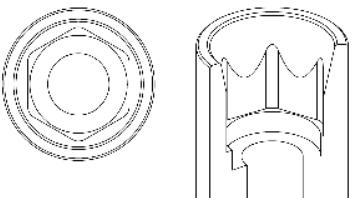

COMPATIBLE with 0170

STANDARD DYNAMIC TIBASE®											
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
0,3 mm		mm		mm		mm		mm		mm	
R	31.322.170.01-2	38°	-	-	-	-	-	-	-	-	-
NR	31.312.170.01-2		-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®		
GINGIVAL HEIGHT		
α_s	α_s	α_s
CH=5mm	CH=7mm	CH=9mm
-	-	-
-	-	-


DYNAMIC μ SCANBODY (LAB/CLIN)		DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
-	-	-	-	-
-	-	-	-	-

COBALT-CHROME	α_{dp}
-	-

DYNAMIC MILLING TOOL	SHANK	α_{di}
33.390.754.01-2	3	25°
33.490.754.01-2	4	
33.690.754.01-2	6	

DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.316.079.02-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

STRAIGHT SCREW	SCREWDRIVER Hex. 1.20
ANALOG	30.410.006.01-2



LIBRARY CODES	
STANDARD LIBRARY	
LAB SCANBODY	DAS_E_0170
DYNAMIC μ SCANBODY (LAB/CLIN)	-

CAPTIVE SCREW LIBRARY	
LAB SCANBODY	-
DYNAMIC μ SCANBODY (LAB/CLIN)	-
	-

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height
IG= Adaptor (3mm)
 α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_d = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation
R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

COMPATIBLE with 0171

STANDARD DYNAMIC TIBASE®											
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
0,3 mm		mm		mm		mm		mm		mm	
R	31.323.171.01-2	35°	-	-	-	-	-	-	-	-	-
NR	31.313.171.01-2		-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®		
GINGIVAL HEIGHT		
α_s	α_s	α_s
CH=5mm	CH=7mm	CH=9mm
-	-	-
-	-	-


DYNAMIC μ SCANBODY (LAB/CLIN)		DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
-	-	-	-	-
-	-	-	-	-

COBALT-CHROME	α_{dp}
-	-

DYNAMIC MILLING TOOL	SHANK	α_{di}
33.390.754.01-2	3	25°
33.490.754.01-2	4	
33.690.754.01-2	6	

DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.316.079.02-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

STRAIGHT SCREW	SCREWDRIVER Hex. 1.20
ANALOG	30.412.001.01-2

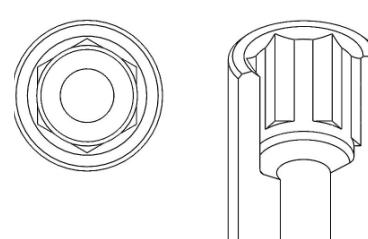

LIBRARY CODES	
STANDARD LIBRARY	
LAB SCANBODY	DAS_E_0171
DYNAMIC μ SCANBODY (LAB/CLIN)	-

CAPTIVE SCREW LIBRARY	
LAB SCANBODY	-
DYNAMIC μ SCANBODY (LAB/CLIN)	-
	-

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height
 α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_d = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation
R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

COMPATIBLE with 0178

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
1,5 mm				mm				mm				mm			
R	31.320.178.01-2	45°	-	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.310.178.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®		
GINGIVAL HEIGHT		
α_s	α_s	α_s
CH=5mm	CH=7mm	CH=9mm
-	-	-
-	-	-


DYNAMIC μ SCANBODY (LAB/CLIN)		DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
-	-	-	-	-
-	-	-	-	-

DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.316.080.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

STRAIGHT SCREWS			
STRAIGHT SCREW	SCREWDRIVER	-	ANALOG LAB SCANBODY
-	-	-	30.410.006.01-2

LIBRARY CODES	
STANDARD LIBRARY	
LAB SCANBODY	DAS_E_0178
DYNAMIC μ SCANBODY (LAB/CLIN)	-
SCAPTURE SCREW LIBRARY	
LAB SCANBODY	-
DYNAMIC μ SCANBODY (LAB/CLIN)	-

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height
 α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation
R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

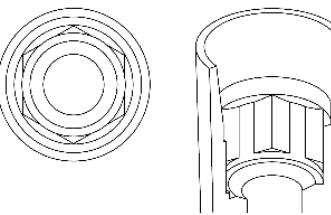

COMPATIBLE with 0181

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
mm				mm				mm				mm			
R	-	-	-	-	-	-	-	-	-	-	-	-	-	-	-
NR	-	-	-	-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®		
GINGIVAL HEIGHT		
α_s	α_s	α_s
0,4 mm	CH=5mm	CH=7mm
-	-	-


DYNAMIC μ SCANBODY (LAB/CLIN)		DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL	SCANLOG
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME
52.408.112.01-2	8				
		50.312.181.01-2	43.620.411.01-2	-	
-	-				-

DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.318.043.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

STRAIGHT SCREWS			
STRAIGHT SCREW	SCREWDRIVER	-	ANALOG LAB SCANBODY
-	-	-	-

LIBRARY CODES	
STANDARD LIBRARY	
LAB SCANBODY	DAS_E_0181
DYNAMIC μ SCANBODY (LAB/CLIN)	-
SCAPTURE SCREW LIBRARY	
LAB SCANBODY	-
DYNAMIC μ SCANBODY (LAB/CLIN)	-
SCANLOG	DAS_SA_0101

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height
 α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation
R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

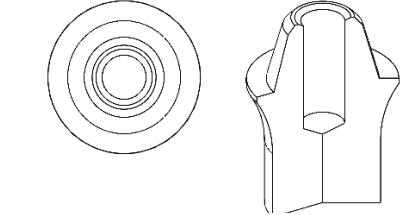

COMPATIBLE with 0186

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
1,2 mm		2,5 mm		3,5 mm		mm		mm		mm		mm		mm	
R	31.323.186.01-2	40°	30°	31.323.186.02-2	20°	18°	31.323.186.03-2	15°	-	-	○	○	-	○	○
NR	31.313.186.01-2			31.313.186.02-2			31.313.186.03-2			-	○	○	-	○	○

DYNAMIC 3TIBASE®		
GINGIVAL HEIGHT		
α_s	α_s	α_s
CH=5mm	CH=7mm	CH=9mm
-	-	-
-	-	-

DYNAMIC µSCANBODY (LAB/CLIN)		DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
-	-	-	-	-
-	-	-	-	-
-	-	-	-	-

DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.316.084.02-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32


STRAIGHT SCREWS			
STRAIGHT SCREW	SCREWDRIVER	-	ANALOG LAB SCANBODY
-	-	-	30.413.002.01-2

LIBRARY CODES	
STANDARD LIBRARY	
LAB SCANBODY	DAS_E_0186
DYNAMIC µSCANBODY (LAB/CLIN)	-
CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_C_E_0186
DYNAMIC µSCANBODY (LAB/CLIN)	-

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

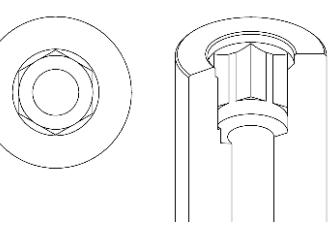

COMPATIBLE with 0187

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
0,3 mm		0,5 mm		1 mm		mm		mm		mm		mm		mm	
R	31.322.009.01-2	45°	25°	31.322.009.02-2	25°	25°	25°	31.322.009.03-2	25°	-	-	-	-	-	-
NR	31.312.009.01-2			31.312.009.02-2				31.312.009.03-2				-	-	-	-

DYNAMIC 3TIBASE®		
GINGIVAL HEIGHT		
α_s	α_s	α_s
CH=5mm	CH=7mm	CH=9mm
-	-	-
-	-	-

DYNAMIC µSCANBODY (LAB/CLIN)		DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
52.410.114.01-2	10		43.621.410.01-2	
		50.312.187.01-2	43.624.410.01-2	34.612.187.01-2
52.412.114.01-2	12		43.630.410.01-2	

DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.316.059.01-2		-	43.618.201.01-2
			18
			43.624.201.01-2
			24
			43.632.201.01-2
			32


STRAIGHT SCREWS			
STRAIGHT SCREW	SCREWDRIVER	-	ANALOG LAB SCANBODY
-	-	-	30.412.001.01-2

LIBRARY CODES	
STANDARD LIBRARY	
LAB SCANBODY	DAS_E_0187
DYNAMIC µSCANBODY (LAB/CLIN)	DAS_I_10_0187
CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_C_E_0187
DYNAMIC µSCANBODY (LAB/CLIN)	DAS_C_I_10_0187
	DAS_C_I_12_0187

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

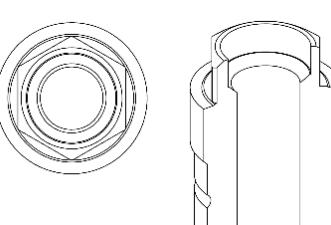

COMPATIBLE with 0196

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
1,2 mm				2 mm				mm				mm			
R	31.320.196.01-2	40°	-	31.320.196.02-2	25°	-	-	-	o	o	-	o	o	-	o
NR	31.310.196.01-2			31.310.196.02-2			-	-	o	o	-	o	o	-	o

DYNAMIC 3TIBASE®		
GINGIVAL HEIGHT		
α_s	α_s	α_s
CH=5mm	CH=7mm	CH=9mm
-	-	-
-	-	-

DYNAMIC µSCANBODY (LAB/CLIN)		DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
-	-	-	-	-
-	-	-	-	-
-	-	-	-	-

DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.316.086.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

STRAIGHT SCREWS			
STRAIGHT SCREW	SCREWDRIVER	-	ANALOG LAB SCANBODY
-	-	-	30.410.006.01-2


LIBRARY CODES	
STANDARD LIBRARY	
LAB SCANBODY	DAS_E_0196
DYNAMIC µSCANBODY (LAB/CLIN)	-
NR	-

CAPTIVE SCREW LIBRARY	
LAB SCANBODY	-
DYNAMIC µSCANBODY (LAB/CLIN)	-
NR	-

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

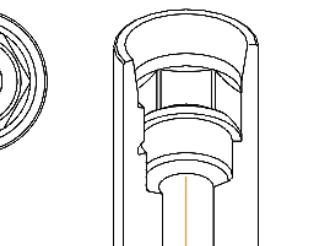

COMPATIBLE with 0197

STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
1,2 mm				2 mm				mm				mm			
R	31.322.197.01-2	35°	-	31.322.197.02-2	20°	-	-	-	-	-	-	-	-	-	-
NR	31.312.197.01-2			31.312.197.02-2			-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®		
GINGIVAL HEIGHT		
α_s	α_s	α_s
CH=5mm	CH=7mm	CH=9mm
-	-	-
-	-	-

DYNAMIC µSCANBODY (LAB/CLIN)		DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
-	-	-	-	-
-	-	-	-	-
-	-	-	-	-

DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.316.086.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

STRAIGHT SCREWS			
STRAIGHT SCREW	SCREWDRIVER	-	ANALOG LAB SCANBODY
-	-	-	30.412.001.01-2


LIBRARY CODES	
STANDARD LIBRARY	
LAB SCANBODY	DAS_E_0197
DYNAMIC µSCANBODY (LAB/CLIN)	-
NR	-

CAPTIVE SCREW LIBRARY	
LAB SCANBODY	-
DYNAMIC µSCANBODY (LAB/CLIN)	-
NR	-

LIBRARY OPTIONS
GH = Gingival Height
CH = Cement Height

α_s = Standard maximum angulation
 α_c = Captive maximum angulation
 α_{di} = Direct to implant maximum angulation
 α_{dp} = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

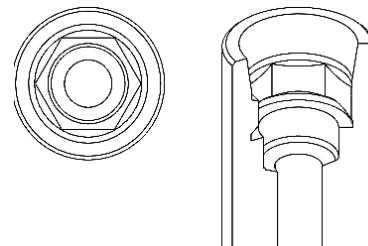

COMPATIBLE with 0198


STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
1,2 mm				mm				mm				mm			
R	31.324.198.01-2	40°	-	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.314.198.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®		
GINGIVAL HEIGHT		
α_s	α_s	α_s
CH=5mm	CH=7mm	CH=9mm
-	-	-
-	-	-

DYNAMIC μ SCANBODY (LAB/CLIN)		DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
-	-	-	-	-
-	-	-	-	-
-	-	-	-	-

DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.316.086.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

LIBRARY CODES	
STANDARD LIBRARY	
LAB SCANBODY	DAS_E_0198
DYNAMIC μ SCANBODY (LAB/CLIN)	-
CAPTIVE SCREW LIBRARY	
LAB SCANBODY	-
DYNAMIC μ SCANBODY (LAB/CLIN)	-

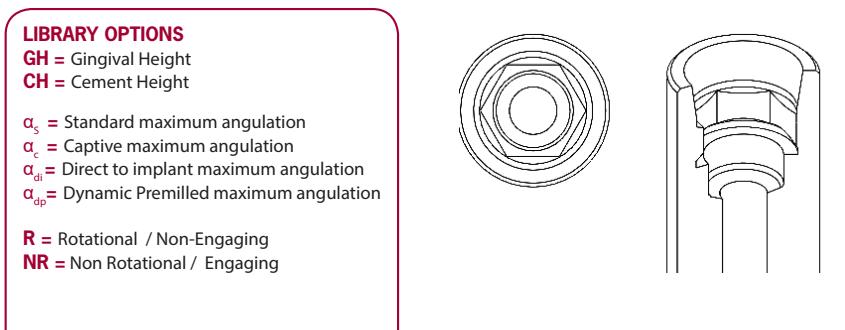

COMPATIBLE with 0205


STANDARD DYNAMIC TIBASE®															
GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c	GINGIVAL HEIGHT		α_s	α_c
0,3 mm				mm				mm				mm			
R	31.322.205.01-2	45°	-	-	-	-	-	-	-	-	-	-	-	-	-
NR	-			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®		
GINGIVAL HEIGHT		
α_s	α_s	α_s
CH=5mm	CH=7mm	CH=9mm
-	-	-
-	-	-

DYNAMIC μ SCANBODY (LAB/CLIN)		DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
-	-	-	-	-
-	-	-	-	-
-	-	-	-	-

DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.317.040.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32



LIBRARY CODES	
STANDARD LIBRARY	
LAB SCANBODY	DAS_E_0205
DYNAMIC μ SCANBODY (LAB/CLIN)	-
CAPTIVE SCREW LIBRARY	
LAB SCANBODY	-
DYNAMIC μ SCANBODY (LAB/CLIN)	-

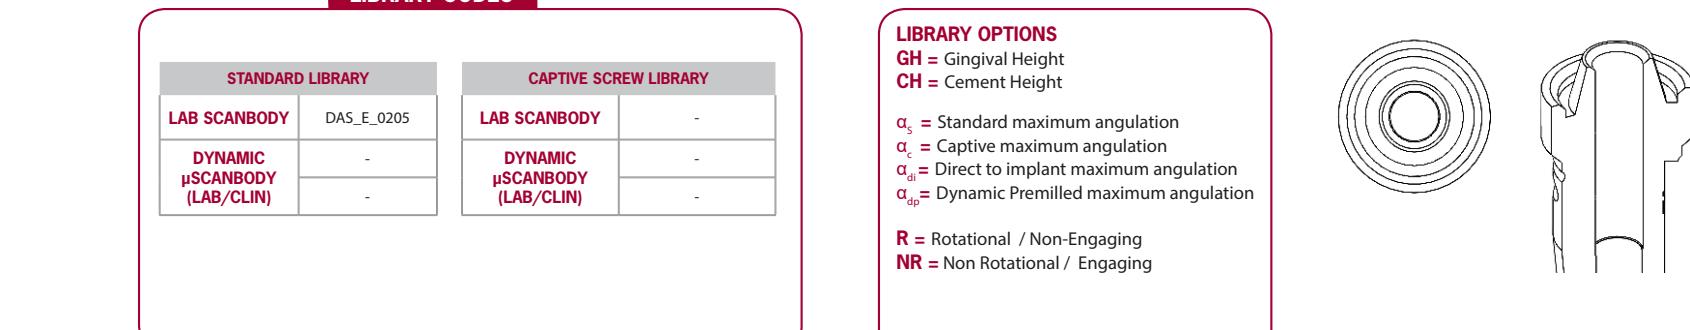

DYNAMIC SCREWS TECHNICAL SPECIFICATIONS

REFERENCE	METRIC	TORQUE	TOTAL LENGTH	THREAD LENGTH	A LENGTH	B LENGTH	C LENGTH	HEAD DIAMETER	SEAT	ANGLE	THREAD ENTRY	CONNECTION
41.312.078.01-2	1,2	15 N·cm	7,8	2,65	6	6,55	1,25	2,3	conical	45°	45° Chamfer	
41.314.039.01-2	1,4	15 N·cm	3,9	1,8	2,1	-	1,8	2,4	straight	-	45° Chamfer	
41.314.040.01-2	1,4	15 N·cm	4	1,85	2	2,78	1,22	2,3	conical	30°	45° Chamfer	
41.314.040.02-2	1,4	15 N·cm	4	1,7	2,25	2,7	1,3	2,3	conical	45°	45° Chamfer	
41.314.043.01-2	1,4	15 N·cm	4,3	1,8	2,03	2,9	1,4	2,3	conical	35°	45° Chamfer	
41.314.045.01-2	1,4	15 N·cm	4,5	2,3	2,5	3,28	1,22	2,3	conical	30°	45° Chamfer	
41.314.046.01-2	1,4	15 N·cm	4,6	2,5	4,6	3,17	1,43	2,3	conical	35°	45° Chamfer	
41.314.052.01-2	1,4	15 N·cm	5,2	2,9	3,4	-	1,8	2,3	straight	-	45° Chamfer	
41.314.064.01-2	1,4	15 N·cm	6,4	2,2	4,21	5,15	1,25	2,3	conical	25°	45° Chamfer	
41.314.064.02-2	1,4	15 N·cm	6,4	2,2	4,65	-	1,75	2,3	straight	-	45° Chamfer	
41.314.067.01-2	1,4	15 N·cm	6,7	2,31	5	5,45	1,25	2,3	conical	45°	45° Chamfer	
41.314.067.02-2	1,4	15 N·cm	6,7	2,5	4,71	5,5	1,2	2,3	conical	35°	45° Chamfer	
41.314.070.01-2	1,4	15 N·cm	7	2,3	5,39	5,65	1,61	2,3	conical	60°	45° Chamfer	
41.314.074.01-2	1,4	15 N·cm	7,4	3,55	5	5,99	1,41	2,3	conical	25°	45° Chamfer	
41.314.076.01-2	1,4	15 N·cm	7,6	2,4	5,9	6,35	1,25	2,3	conical	45°	45° Chamfer	
41.314.080.01-2	1,4	15 N·cm	8	2,1	4,96	6,8	1,2	2,3	conical	15°	45° Chamfer	
41.314.084.01-2	1,4	15 N·cm	8,4	2,5	5,92	6,85	1,55	2,3	conical	35°	45° Chamfer	
41.314.105.01-2	1,4	15 N·cm	10,5	2,31	5	5,45	5,05	2,3	conical	45°	45° Chamfer	
41.316.044.01-2	1,6	20 N·cm	4,4	2,5	2,9	-	1,5	2,3	straight	-	Semi-sphere	
41.316.055.01-2	1,6	20 N·cm	5,5	2,4	2,85	4,2	1,3	2,3	conical	23°	45° Chamfer	
41.316.059.01-2	1,6	20 N·cm	5,9	3	4,4	-	1,5	2,3	straight	-	Semi-sphere	
41.316.071.01-2	1,6	20 N·cm	7,1	2,8	5,2	5,53	1,57	2,3	conical	60°	45° Chamfer	
41.316.072.01-2	1,6	20 N·cm	7,2	3,5	5,2	5,85	1,35	2,3	conical	30°	45° Chamfer	
41.316.073.01-2	1,6	20 N·cm	7,3	2,2	4,87	5,56	1,74	2,3	conical	35°	45° Chamfer	
41.316.074.01-2	1,6	20 N·cm	7,4	2,7	5,5	6	1,4	2,3	conical	45°	45° Chamfer	
41.316.076.01-2	1,6	20 N·cm	7,6	3,6	6,1	-	1,5	2,3	straight	-	Semi-sphere	

HEXALOBULAR

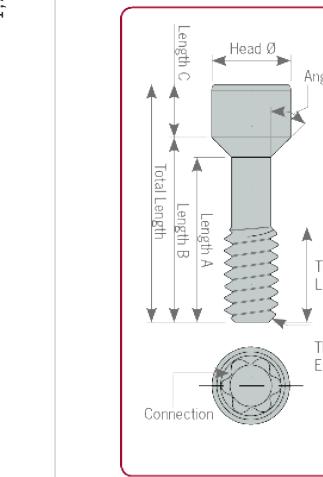
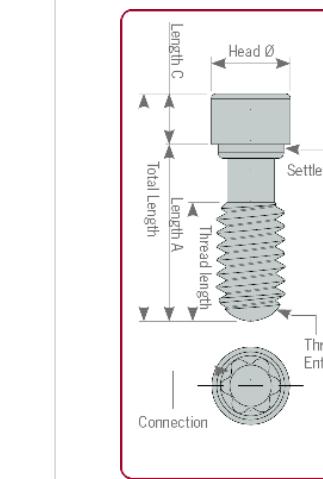


REFERENCE	METRIC	TORQUE	TOTAL LENGTH	THREAD LENGTH	A LENGTH	B LENGTH	C LENGTH	HEAD DIAMETER	SEAT	ANGLE	THREAD ENTRY	CONNECTION
41.316.078.01-2	1,6	20 N·cm	7,8	2	5,36	7,03	0,81	2,3	conical	15°	45° Chamfer	
41.316.079.01-2	1,6	20 N·cm	7,9	2,30	5,42	6,60	1,3	2,3	conical	20°	45° Chamfer	
41.316.079.02-2	1,6	20 N·cm	7,9	3,9	6,3	-	1,6	2,3	straight	-	45° Chamfer	
41.316.080.01-2	1,6	20 N·cm	8	3,14	6,3	6,51	1,49	2,3	conical	60°	45° Chamfer	
41.316.081.01-2	1,6	20 N·cm	8,1	3	6,35	6,72	1,38	2,3	conical	45°	45° Chamfer	
41.316.084.01-2	1,6	20 N·cm	8,4	3,5	6,8	-	1,6	2,3	straight	-	Semi-sphere	
41.316.084.02-2	1,6	20 N·cm	8,4	2,7	5,85	6,85	1,55	2,3	conical	30°	45° Chamfer	
41.316.086.01-2	1,6	20 N·cm	8,6	3	7,2	-	1,4	2,3	straight	-	45° Chamfer	
41.316.094.01-2	1,6	20 N·cm	9,4	2,9	7,65	8	1,4	2,3	conical	45°	45° Chamfer	
41.316.094.02-2	1,6	20 N·cm	9,4	2,9	7,9	-	1,5	2,3	straight	-	45° Chamfer	
41.316.108.01-2	1,6	20 N·cm	10,8	2	5,36	7,03	0,81	2,3	conical	15°	45° Chamfer	
41.316.118.01-2	1,6	20 N·cm	11,8	3,6	6,1	-	5,7	2,3	straight	-	Semi-sphere	
41.316.124.01-2	1,6	20 N·cm	12,4	2,2	4,74	5,56	5,24	2,3	conical	35°	45° Chamfer	
41.316.132.01-2	1,6	20 N·cm	13,2	2,9	7,62	8	5,2	2,3	conical	45°	45° Chamfer	
41.317.040.01-2	N1-72	25 N·cm	4	2,1	2,5	-	1,5	2,3	straight	-	45° Chamfer	
41.317.065.01-2	N1-72	25 N·cm	6,5	2,4	4,7	5,18	1,33	2,3	conical	45°	45° Chamfer	
41.317.070.01-2	N1-72	25 N·cm	7	2,2	4,96	5,8	1,2	2,3	conical	30°	45° Chamfer	
41.317.071.01-2	N1-72	25 N·cm	7,1	2,6	5,56	5,65	1,45	2,3	conical	70°	45° Chamfer	
41.317.071.02-2	N1-72	25 N·cm	7,1	2,6	5,6	-	1,5	2,3	straight	-	45° Chamfer	
41.317.073.01-2	N1-72	25 N·cm	7,3	2,5	5,5	5,77	1,53	2,3	conical	60°	45° Chamfer	
41.317.106.01-2	N1-72	25 N·cm	10,6	2,6	5,54	5,65	4,95	2,3	conical	70°	Semi-sphere	
41.318.035.01-2	1,8	25 N·cm	3,5	1,9	1,93	2,2	1,4	2,3	conical	60°	45° Chamfer	
41.318.043.01-2	1,8	25 N·cm	4,3	2	2,52	2,7	1,6	2,3	conical	55°	45° Chamfer	
41.318.044.01-2	1,8	25 N·cm	4,4	2,75	3	-	1,4	2,3	straight	-	Semi-sphere	
41.318.045.01-2	1,8	25 N·cm	4,5	2,3	2,81	2,9	1,6	2,3	conical	70°	45° Chamfer	
41.318.048.01-2	1,8	25 N·cm	4,8	2,8	3,22	3,65	1,15	2,3	conical	30°	Semi-sphere	
41.318.051.01-2	1,8	25 N·cm	5,1	2,7	3,55	3,7	1,4	2,3	conical	60°	45° Chamfer	
41.318.051.02-2	1,8	25 N·cm	5,1	2,7	3,55	3,7	1,4	2,3	conical	45°	45° Chamfer	



DYNAMIC SCREWS TECHNICAL SPECIFICATIONS

REFERENCE	METRIC	TORQUE	TOTAL LENGTH	THREAD LENGTH	A LENGTH	B LENGTH	C LENGTH	HEAD DIAMETER	SEAT	ANGLE	THREAD ENTRY	CONNECTION
41.318.064.01-2	1,8	25 N-cm	6,4	3,45	4,73	5,1	1,3	2,3	conical	35°	45° Chamfer	
41.318.065.01-2	1,8	25 N-cm	6,5	2,8	5	-	1,5	2,3	straight	-	Semi-sphere	
41.318.067.01-2	1,8	25 N-cm	6,7	2,35	5	5,4	1,3	2,3	conical	45°	45° Chamfer	
41.318.068.01-2	1,8	25 N-cm	6,8	4	5,25	5,4	1,4	2,3	conical	60°	45° Chamfer	
41.318.071.01-2	1,8	25 N-cm	7,1	2,6	5,56	5,65	1,45	2,3	conical	70°	45° Chamfer	
41.318.074.01-2	1,8	25 N-cm	7,4	3,8	5,8	6,03	1,6	2,3	conical	50°	45° Chamfer	
41.318.075.01-2	1,8	25 N-cm	7,5	3,3	6,1	-	1,4	2,3	straight	-	Semi-sphere	
41.318.076.01-2	1,8	25 N-cm	7,6	2,52	5,8	6,2	1,4	2,3	conical	45°	45° Chamfer	
41.318.077.01-2	1,8	25 N-cm	7,7	2,5	5,81	1,89	1,2	2,3	conical	30°	45° Chamfer	
41.318.077.02-2	1,8	25 N-cm	7,7	2	6,09	6,35	1,35	2,3	conical	60°	45° Chamfer	
41.318.080.01-2	1,8	25 N-cm	8	4	6,5	-	1,5	2,3	straight	-	45° Chamfer	
41.318.083.01-2	1,8	25 N-cm	8,3	4,25	6,79	6,95	1,35	2,3	conical	60°	45° Chamfer	
41.320.038.01-2	2	25 N-cm	3,81	1,6	3,25	2,35	1,39	2,35	conical	70°	20° Chamfer	
41.320.044.01-2	2	25 N-cm	4,4	2,45	2,45	3,1	1,3	2,3	conical	45°	45° Chamfer	
41.320.047.01-2	2	25 N-cm	4,7	3	3,3	-	1,4	2,3	straight	-	Semi-sphere	
41.320.048.01-2	2	25 N-cm	4,8	2,7	3,3	3,4	1,4	2,3	conical	60°	45° Chamfer	
41.320.050.01-2	2	25 N-cm	5	2,8	3,39	3,6	1,4	2,3	conical	30°	Semi-sphere	
41.320.051.01-2	2	25 N-cm	5,1	3,1	3,6	-	1,5	2,3	straight	-	Semi-sphere	
41.320.060.01-2	2	25 N-cm	6	2,7	4,5	-	1,5	2,3	straight	-	Semi-sphere	
41.320.065.01-2	2	25 N-cm	6,5	2,7	5	-	1,5	2,3	straight	-	45° Chamfer	
41.320.067.01-2	2	25 N-cm	6,7	2,3	3,65	5,68	1,02	2,58	conical	15°	45° Chamfer	
41.320.068.01-2	2	25 N-cm	6,8	4,4	5,3	5,4	1,4	2,3	conical	60°	45° Chamfer	
41.320.070.01-2	2	25 N-cm	7	3	5,6	-	1,4	2,3	straight	-	Semi-sphere	
41.320.074.01-2	2	25 N-cm	7,4	3,3	6	-	1,4	2,3	straight	-	Semi-sphere	
41.320.075.01-2	2	25 N-cm	7,5	2,75	5,93	6,18	1,32	2,3	conical	35°	45° Chamfer	

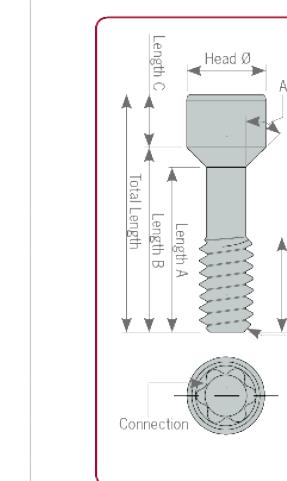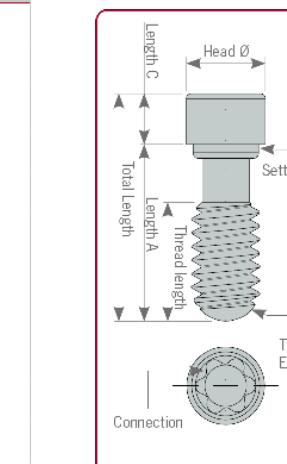

Hexalobular
1,70

REFERENCE	METRIC	TORQUE	TOTAL LENGTH	THREAD LENGTH	A LENGTH	B LENGTH	C LENGTH	HEAD DIAMETER	SEAT	ANGLE	THREAD ENTRY	CONNECTION
41.320.079.01-2	2	25 N-cm	7,9	3,3	6,33	6,5	1,4	2,3	conical	45°	45° Chamfer	
41.320.082.01-2	2	25 N-cm	8,2	4,7	6,7	-	1,5	2,4	straight	-	Semi-sphere	
41.320.090.01-2	2	25 N-cm	9	4	7,5	-	1,5	2,3	straight	-	Semi-sphere	
41.320.094.01-2	2	25 N-cm	9,4	3	7,85	8	1,4	2,3	conical	45°	45° Chamfer	
41.320.094.02-2	0	25 N-cm	9,4	3	7,9	-	1,5	2,3	straight	-	45° Chamfer	
41.320.117.01-2	2	25 N-cm	11,7	2,75	5,9	6,18	5,52	2,3	conical	35°	Semi-sphere	
41.320.125.01-2	2	25 N-cm	12,5	3,3	6,33	6,5	6	2,3	conical	45°	45° Chamfer	
41.325.054.01-2	2,5	25 N-cm	5,4	3,8	4,1	-	1,3	2,85	straight	-	Semi-sphere	
41.325.067.01-2	2,5	25 N-cm	6,7	4,6	5,1	-	1,6	2,85	straight	-	Semi-sphere	

Hexalobular
1,70

DYNAMIC SCREWDRIVER & DYNAMIC SCREWS

Dynamic Screwdrivers



Screwdriver with hexalobular head, exclusively to the 3.0 Dynamic Abutment® system.



Lengths:
18, 24, 32mm.

Dynamic Screws are used with the Dynamic TiBase® or milled structures with an angled screw channel.
Made of Titanium grade V.

High Dynamic Screw Dynamic Screw

STRAIGHT SCREWS TECHNICAL SPECIFICATIONS

REFERENCE	METRIC	TORQUE	TOTAL LENGTH	THREAD LENGTH	A LENGTH	B LENGTH	C LENGTH	HEAD DIAMETER	SEAT	ANGLE	THREAD ENTRY	CONNECTION
40.312.003.01-2	1,2	15 N-cm	7,85	2,7	6,19	6,55	1,3	1,9	conical	45°	45° Chamfer	Hex. 1,20
40.314.003.01-2	1,4	15 N-cm	3,9	1,91	2,1	-	1,8	2,4	straight	-	45° Chamfer	Hex. 1,20
40.314.003.02-2	1,4	15 N-cm	4	2	2,2	-	1,8	2,3	straight	-	45° Chamfer	Hex. 1,20
40.314.003.03-2	1,4	15 N-cm	7,6	2,4	6,05	6,3	1,3	1,9	conical	45°	45° Chamfer	Hex. 1,20
40.314.003.04-2	1,4	15 N-cm	7,5	2,5	5,45	5,7	1,8	1,85	conical	45°	45° Chamfer	Hex. 1,20
40.314.004.01-2	1,4	15 N-cm	6,3	1,7	4,6	5,1	1,2	2,1	conical	25°	30° Chamfer	Hex. 1,25
40.314.004.02-2	1,4	15 N-cm	8,4	2,5	5,99	6,7	1,7	2	conical	35°	45° Chamfer	Hex. 1,25
40.314.004.03-2	1,4	15 N-cm	4,3	1,8	2,3	-	2	2	straight	-	45° Chamfer	Hex. 1,25
40.314.005.01-2	1,4	15 N-cm	7,6	3,55	5,17	6	1,6	2,15	conical	25°	45° Chamfer	Hex. 1,27
40.314.005.02-2	1,4	15 N-cm	7,5	2,5	5,5	5,7	1,7	2,1	conical	60°	45° Chamfer	Hex. 1,27
40.314.007.01-2	1,4	15 N-cm	4	1,8	2,01	2,8	1,2	2,2	conical	35°	45° Chamfer	Torx T6
40.314.007.02-2	1,4	15 N-cm	7	2,1	4,75	2,25	0,8	2,1	conical	15°	45° Chamfer	Torx T6
40.314.008.01-2	1,4	15 N-cm	3,5	1,8	2,1	-	1,4	2	straight	-	45° Chamfer	Unigrip
40.314.008.02-2	1,4	15 N-cm	6,7	2,5	4,87	5,3	1,4	1,8	conical	35°	45° Chamfer	Unigrip
40.314.012.01-2	1,4	15 N-cm	4,5	1,7	2,01	2,4	2,1	2,15	conical	45°	45° Chamfer	Star 1,50
40.314.014.01-2	1,4	15 N-cm	4,45	2	2,48	-	1,97	2,16	straight	-	45° Chamfer	Hex. 1,19
40.316.002.01-2	1,6	20 N-cm	7	2,79	4,86	5,44	1,56	2,3	conical	45°	45° Chamfer	Sq. 1,30
40.316.002.02-2	1,6	20 N-cm	9,3	3,3	7,3	-	2	2,3	straight	-	Semi-sphere	Sq. 1,30
40.316.003.01-2	1,6	20 N-cm	8,4	2,5	6,6	-	1,8	2	straight	-	45° Chamfer	Hex. 1,20
40.316.003.02-2	1,6	20 N-cm	10,2	2	7,88	8,2	2	2,2	conical	45°	45° Chamfer	Hex. 1,20
40.316.004.01-2	1,6	20 N-cm	8,6	2,7	6,16	6,9	1,7	2	conical	30°	45° Chamfer	Hex. 1,25
40.316.004.02-2	1,6	20 N-cm	8,8	3	6,73	6,8	1,8	2,1	conical	45°	45° Chamfer	Hex. 1,25
40.316.004.03-2	1,6	20 N-cm	6,9	2,2	5,02	5,2	1,7	1,92	conical	60°	45° Chamfer	Hex. 1,25
40.316.005.01-2	1,6	20 N-cm	7,5	3,6	5,33	5,85	1,65	2,15	conical	30°	45° Chamfer	Hex. 1,27
40.316.005.02-2	1,6	20 N-cm	8,2	3,03	6,25	-	2	2,33	straight	-	45° Chamfer	Hex. 1,27
40.316.005.04-2	1,6	20 N-cm	10,5	2,9	8,15	8,4	2,1	2,1	conical	45°	45° Chamfer	Hex. 1,27
40.316.005.05-2	1,6	20 N-cm	7,6	2,7	5,21	5,5	2,1	2,1	conical	60°	45° Chamfer	Hex. 1,27

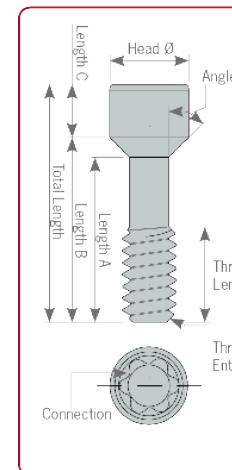
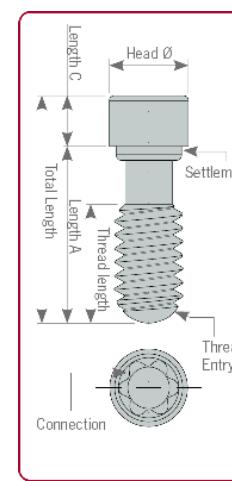


REFERENCE	METRIC	TORQUE	TOTAL LENGTH	THREAD LENGTH	A LENGTH	B LENGTH	C LENGTH	HEAD DIAMETER	SEAT	ANGLE	THREAD ENTRY	CONNECTION
40.316.005.06-2	1,6	20 N-cm	3,6	1,8	2,2	-	1,4	2,1	straight	-	45° Chamfer	Hex. 1,27
40.316.005.07-2	1,6	20 N-cm	8,8	2,85	6,73	6,9	1,9	2,15	conical	60	45° Chamfer	Hex. 1,27
40.316.005.08-2	1,6	20 N-cm	9	3,9	0	6,9	2,1	2,18	conical	45°	45° Chamfer	Hex. 1,27
40.316.0 07.01-2	1,6	20 N-cm	7,9	2	5,72	6,9	2,18	2,18	conical	15°	45° Chamfer	Torx T6
40.316.008.01-2	1,6	20 N-cm	7	2,7	5,15	-	1,8	2,3	straight	-	45° Chamfer	Unigrip
40.316.008.02-2	1,6	20 N-cm	7,3	2,7	5,15	5,9	1,4	2,2	conical	35°	45° Chamfer	Unigrip
40.316.012.01-2	1,6	20 N-cm	8	2,65	5,53	6	2	2,15	conical	45°	45° Chamfer	Star 1,50
40.316.014.01-2	1,6	20 N-cm	7,9	2,3	5,42	6,46	1,44	2,2	conical	20°	45° Chamfer	Hex. 1,19
40.317.002.01-2	N1-72	25 N-cm	8,17	3	5,31	5,87	2,3	2,4	conical	45°	45° Chamfer	Sq. 1,30
40.317.004.01-2	N1-72	25 N-cm	7,6	2,8	5,6	5,76	1,84	2,3	conical	70°	45° Chamfer	Hex. 1,27
40.317.004.02-2	N1-72	25 N-cm	7,52	2,2	5,12	5,773	1,75	2,1	conical	30°	45° Chamfer	Hex. 1,25
40.317.005.01-2	N1-72	25 N-cm	7,6	2,5	5,19	5,42	2,18	2,2	conical	60°	45° Chamfer	Hex. 1,27
40.317.005.02-2	N1-72	25 N-cm	7,2	2,4	4,73	5,25	1,95	2,4	conical	45°	45° Chamfer	Hex. 1,27
40.318.002.01-2	1,8	25 N-cm	7	3,2	5,2	-	1,8	2,5	straight	-	45° Chamfer	Sq. 1,30
40.318.002.02-2	1,8	25 N-cm	8,3	2,6	6,6	-	1,7	2,45	straight	-	45° Chamfer	Sq. 1,30
40.318.003.01-2	1,8	25 N-cm	6,8	3,3	5,2	-	1,6	2,3	straight	-	45° Chamfer	Hex. 1,20
40.318.003.02-2	1,8	25 N-cm	8	3,6	6	-	2	2,1	straight	-	45° Chamfer	Hex. 1,20
40.318.004.01-2	1,8	25 N-cm	7,2	4,47	2,3	6,2	1	2,4	conical	30°	45° Chamfer	Hex. 1,25
40.318.004.02-2	1,8	25 N-cm	9,8	5,094	8,3	8,8	1	2,4	conical	30°	45° Chamfer	Hex. 1,25
40.318.004.03-2	1,8	25 N-cm	7,65	3,3	5,17	5,75	1,9	2,4	conical	35°	45° Chamfer	Hex. 1,25
40.318.005.01-2	1,8	25 N-cm	4,5	2,3	2,8	2,9	1,6	2,35	conical	70°	45° Chamfer	Hex. 1,27
40.318.005.02-2	1,8	25 N-cm	7,6	3,8	5,8	6,05	1,55	2,35	conical	50°	45° Chamfer	Hex. 1,27
40.318.006.01-2	1,8	25 N-cm	6	3,18	3,5	3,85	2,15	2,4	conical	45°	45° Chamfer	Hex. 1,50
40.318.007.01-2	1,8	25 N-cm	9,1	4,25	7,22	7,45	1,65	2,18	conical	60°	45° Chamfer	Torx T6
40.318.008.01-2	1,8	25 N-cm	8,3	2,5	6,5	-	1,8	2,45	straight	-	45° Chamfer	Unigrip
40.318.012.01-2	1,8	25 N-cm	7,25	2,4	4,93	5,25	2	2,15	conical	45°	45° Chamfer	Sq. 1,50



STRAIGHT SCREWS TECHNICAL SPECIFICATIONS

REFERENCE	METRIC	TORQUE	TOTAL LENGTH	THREAD LENGTH	A LENGTH	B LENGTH	C LENGTH	HEAD DIAMETER	SEAT	ANGLE	THREAD ENTRY	CONNECTION
40.318.013.01-2	1,8	25 N·cm	8	2,5	6,01	6,7	1,3	2,2	conical	30°	45° Chamfer	Hex. 1,00
40.320.002.01-2	2	30 N·cm	5	3,06	3,26	3,5	1,5	2,49	conical	45°	45° Chamfer	Sq. 1,30
40.320.002.02-2	2	30 N·cm	7,45	3	5,7	5,9	1,5	2,4	conical	45°	45° Chamfer	Sq. 1,30
40.320.002.03-2	2	30 N·cm	10,2	3,15	8,4	-	1,8	2,45	straight	-	45° Chamfer	Sq. 1,30
40.320.003.01-2	2	30 N·cm	4,7	2,7	3,33	-	1,37	2,35	straight	-	45° Chamfer	Hex. 1,20
40.320.003.02-2	2	30 N·cm	7	3,25	5	-	2	2,4	straight	-	45° Chamfer	Hex. 1,20
40.320.003.03-2	2	30 N·cm	7,9	3,7	5,55	6,05	1,85	2,4	conical	45°	45° Chamfer	Hex. 1,20
40.320.003.04-2	2	30 N·cm	8,4	2,75	5,68	6,35	2,05	2,3	conical	45°	45° Chamfer	Hex. 1,20
40.320.003.05-2	2	30 N·cm	4,8	3,3	3,65	3,9	0,9	2,45	conical	45°	45° Chamfer	Hex. 1,20
40.320.005.01-2	2	30 N·cm	7,6	3,7	6	-	1,6	2,4	straight	-	45° Chamfer	Hex. 1,27
40.320.005.02-2	2	30 N·cm	10,3	4	8,3	-	2	2,45	straight	-	45° Chamfer	Hex. 1,27
40.320.005.03-2	2	30 N·cm	10,3	3,5	8,3	-	2	2,33	straight	-	45° Chamfer	Hex. 1,27
40.320.005.04-2	2	30 N·cm	10,5	3,06	8,15	8,4	2,1	2,5	conical	45°	45° Chamfer	Hex. 1,27
40.320.007.01-2	2	30 N·cm	6,7	2,25	3,59	5,7	1	2,58	conical	15°	45° Chamfer	Torx T6
40.320.007.02-2	2	30 N·cm	7,4	3,3	6	-	1,4	2,3	straight	-	Semi-sphere	Torx T6
40.320.007.03-2	2	30 N·cm	7,6	3	6,1	6,3	1,3	2,4	conical	45°	Semi-sphere	Torx T6
40.320.007.04-2	2	30 N·cm	4,5	2,96	3,21	3,5	1	2,45	conical	45°	45° Chamfer	Torx T6
40.320.008.01-2	2	30 N·cm	7	3,25	5	-	2	2,4	straight	-	45° Chamfer	Unigrip
40.320.008.02-2	2	30 N·cm	7,3	3	5,8	6,2	1,1	2,5	conical	35°	45° Chamfer	Unigrip
40.320.008.03-2	2	30 N·cm	10	3,6	8,5	-	1,5	2,45	straight	-	45° Chamfer	Unigrip
40.325.002.01-2	2,5	30 N·cm	7,41	3,5	4,75	5,29	2,12	2,87	conical	45°	Semi-sphere	Sq . 1,30
40.325.008.01-2	2,5	30 N·cm	7	2,8	5,6	-	1,4	3,4	straight	-	45° Chamfer	Unigrip

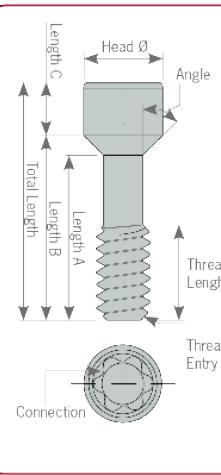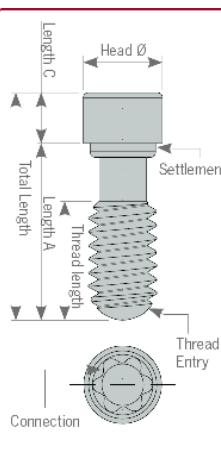

SCREWDRIVERS & STRAIGHT SCREWS

Screwdrivers


REF: 43.601.103.02-2 Hex 1.20mm	REF: 43.601.105.01-2 Hex. 1.27mm
REF: 43.601.102.01-2 Squa. 1.30mm	REF: 43.601.108.01-2 Unigrip
REF: 43.601.104.01-2 Hex 1.25mm	REF: 43.601.107.01-2 Torx T6




Straight Screws

DYNAMIC SYSTEM SCANBODIES AND COLORS ACCORDING TO COMPATIBILITY

COMPATIBILITY CODE	MAIN COMPATIBILITY	SCANBODY TYPE	ADAPTOR REFERENCE	MIDDLE PIECE	MAGNET SCREW
0002	Biomet 3i Certain RP	HA	52.410.101.01-2		
0007	Astra Evolution 4,2				
0017	MIS C1 RP				
0022	Nobel Biocare Active RP				
0024	Nobel Biocare Branemark RP			N/A	
0030	Osstem Implant TS RP				
0040	Zimmer Screw-Vent 3,5				
0057	Biomet 3i Certain WP				
0064	S&M Outlink 4,1			N/A	
0005	Astra Lilac				
0018	MIS C1 WP				
0041	Zimmer Screw-Vent 4,5				
0052	Bego S/RI 4,5				
0091	Astra Evolution 4,8				
0001	Biomet 3i Certain NP	HB	52.410.102.01-2		
0004	Astra Aqua				
0021	Nobel Biocare Active NP				
0023	Nobel Biocare Branemark NP				
0029	Osstem Implant TS Mini				
0038	Xive S 3,4				
0083	Klockner Vega RV				

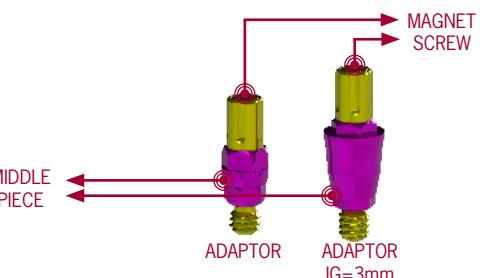


COMPATIBILITY CODE	MAIN COMPATIBILITY	SCANBODY TYPE	REFERENCE	ADAPTOR	MAGNET SCREW
0003	Biomet 3i Osseotite NP	HD	52.410.104.01-2	N/A	
0015	Megagen AnyRidge RP				
0031	S&M Premium Khono 3,3				
0006	Astra Evolution 3,6	HE	52.410.105.01-2		
0019	MIS M4 NP				
0044	Keystone Prima NP				
0075	Ankylos				
0082	Klockner Vega NV				
0008	Astra Evolution Uni Abutment			HF	52.408.113.01-2
0009	BTI External Connection NP	HG	52.410.114.01-2	N/A	
0039	Xive S 3,8				
0187	Bego Mini			N/A	
0049	Bego RS/RSX 3	HH	52.410.116.01-2		
0050	Bego S/RI 3,25-3,75				
0085	Xive S 4,5				
0125	Medentis ICX-Tempplant 4,1				
0167	Lasak Bionoq QR				
0169	Alphabio Conical Standard Connection				
0051	Bego S/RI 4,1	HJ	52.410.118.01-2		
0045	Keystone Prima RP				
0058	Biomet 3i Osseotite WP			N/A	
0032	S&M Premium Khono 3,80	HK	52.410.120.01-2		
0065	S&M Premium Khono 4,25				

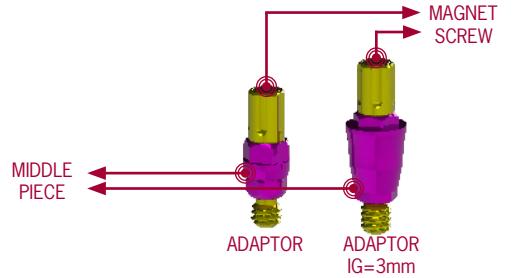


DYNAMIC SYSTEM SCANBODIES AND COLORS ACCORDING TO COMPATIBILITY

COMPATIBILITY CODE	MAIN COMPATIBILITY	SCANBODY TYPE	REFERENCE	ADAPTOR	MAGNET SCREW	
0060	BTI External Connection WP	HM	52.410.122.01-2	N/A		
0047	Neoss ProActive 3,4		52.409.123.01-2			
0048	Neoss ProActive 4,1					
0151	BTI Multi-IM Universal RP			N/A		
0080	Zimmer Screw-Vent 5,7	HO	52.410.124.01-2			
0046	Keystone Prima WP		52.410.125.01-2			
0061	Nobel Biocare Branemark WP			N/A		
0124	Nobel Biocare Active WP					
0081	Bego S/RI 5,50	HR	52.410.126.01-2			
0014	DIO UF NP		52.410.128.01-2			
0090	Astra Evolution 3,0					
0102	Biohorizons 3,0					
0109	Astra Yellow	HS				
0136	Alphabio Conical Hex. Connection					
0159	Nobel Biocare Active 3,0					
0164	Biotech Dental Kontakt 3.0					
0092	Astra Evolution 5,4	HT	52.410.129.01-2			
0025	Nobel Biocare Multi Unit RP		52.410.111.01-2	N/A		
0020	MIS Multi Unit St	MA	52.408.112.01-2	N/A		
0025	Nobel Biocare Multi Unit RP			N/A		
0163	Anthogyr Multi-Unit 4,8			N/A		
0181	Paltop MU			N/A		

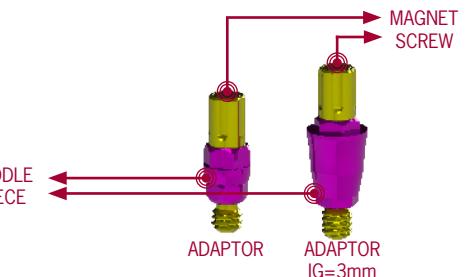


COMPATIBILITY CODE	MAIN COMPATIBILITY	SCANBODY TYPE	REFERENCE	ADAPTOR	MAGNET SCREW
0037	Straumann Internal Octagon 4,8	OA	52.410.110.01-2		
0074	Straumann Synocta RP			N/A	
0096	Straumann Internal Octagon 6,5				
0054	Klockner Essential Cone 4,5	OB	52.410.119.01-2		
0016	MIS C1 NP	SA	52.410.106.01-2		
0033	Straumann Bone Level NP				
0035	Straumann Bone Level RP				
0010	BTI Internal Connection RP	SB	52.410.107.01-2		
0160	Straumann Tissue Level NNC	SC	52.410.115.01-2		
0011	Camlog Screw-Line 3,8	TA	52.410.108.01-2		
0026	Nobel Biocare Replace NP				
0120	Conelog 3,8				
0012	Camlog Screw-Line 4,3	TB	52.410.109.01-2		
0027	Nobel Biocare Replace RP				
0028	Nobel Biocare Replace WP				
0121	Conelog 4,3	TC	52.410.130.01-2		
0129	Nobel Biocare Replace 6,0				
0149	Anthogyr Axiom REG/PX XNP	TD	52.410.132.01-2		
0162	Anthogyr Axiom REG/PX WP				
0161	Anthogyr Axiom REG/PX RP				
0165	Biotech Dental Kontakt RP				

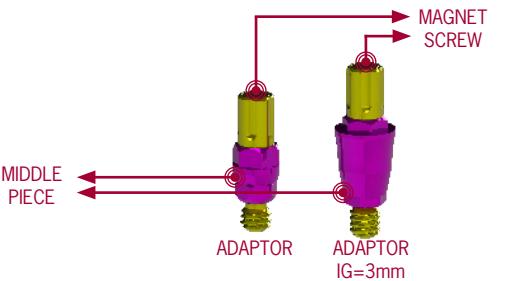

DYNAMIC MILLING TOOL SPECIFICATIONS

MAIN COMPATIBILITY	REFERENCE	CUTTING DIAMETER	SEAT	CUTTING LENGTH	USEFUL LENGTH (max. drilling depth)	STEM CUTTING DIAMETER	SUPPORT DIAMETER (SHANK)	TOTAL LENGTH
		\varnothing_c	Lc	Lu	\varnothing_v	\varnothing_s	Lt	
ASTRA EVOLUTION 3.0 BEGO RS/RX 3	33.325.472.01-2	1,4	25	0,4	4,7	0,5	3	50
	33.425.472.01-2	1,4	25	0,4	4,7	0,5	4	50
	33.625.472.01-2	1,4	25	0,4	4,7	0,5	6	50
MEDENTIS ICX TEMPLANT 4.1 STRAUMANN BONE LEVEL NP STRAUMANN BONE LEVEL RP STRAUMANN TISSUE LEVEL NNC	33.315.804.01-2	1,6	15	0,7	8	0,65	3	50
	33.415.804.01-2	1,6	15	0,7	8	0,65	4	50
	33.615.804.01-2	1,6	15	0,7	8	0,65	6	50
ANTHOGYR AXIOM RG/PX XNP ANTHOGYR AXIOM RG/PX RP ANTHOGYR AXIOM RG/PX WP	33.320.704.01-2	1,6	20	0,7	7	0,8	3	50
	33.420.704.01-2	1,6	20	0,7	7	0,8	4	50
	33.620.704.01-2	1,6	20	0,7	7	0,8	6	50
ALPHABIO CONICAL STANDARD CONNECTION ANKYLOS ASTRA EVOLUTION 3.6	33.330.734.01-2	1,6	30	0,7	7,3	0,8	3	50
	33.430.734.01-2	1,6	30	0,7	7,3	0,8	4	50
	33.630.734.01-2	1,6	30	0,7	7,3	0,8	6	50
NOBEL BIOCARE ACTIVE 3.0 NOBEL BIOCARE ACTIVE NP	33.335.754.01-2	1,6	35	0,7	7,5	0,65	3	50
	33.435.754.01-2	1,6	35	0,7	7,5	0,65	4	50
	33.635.754.01-2	1,6	35	0,7	7,5	0,65	6	50
BIOTECH DENTAL KONTAKT 3.0 BIOTECH DENTAL KONTAKT RP CAMLOG SCREW LINE 3,8/4,3 KLOCKNER VEGA NV OSSTEM IMPLANT TS MINI XIVE S 3,4	33.345.804.01-2	1,6	45	0,7	8	0,65	3	50
	33.445.804.01-2	1,6	45	0,7	8	0,65	4	50
	33.645.804.01-2	1,6	45	0,7	8	0,65	6	50
ALPHABIO CONICAL HEX CONNECTION ASTRA YELLOW CONELOG 3,8/4,3 MIS C1 NP MIS M4 NP	33.360.754.01-2	1,6	60	0,7	7,5	0,65	3	50
	33.460.754.01-2	1,6	60	0,7	7,5	0,65	4	50
	33.660.754.01-2	1,6	60	0,7	7,5	0,65	6	50
ASTRA AQUA BIOMET 3I CERTAIN NP	33.390.754.01-2	1,6	90	0,7	7,5	0,65	3	50
	33.490.754.01-2	1,6	90	0,7	7,5	0,65	4	50
	33.690.754.01-2	1,6	90	0,7	7,5	0,65	6	50
ASTRA EVOLUTION 4.2	33.350.775.01-2	1,7	50	0,7	7,7	0,8	3	50
	33.450.775.01-2	1,7	50	0,7	7,7	0,8	4	50
	33.650.775.01-2	1,7	50	0,7	7,7	0,8	6	50
BIOMET 3I CERTAIN RP/WP MEGAGEN ANYRIDGE RP NOBEL BIOCARE BRANEMARK NP NOBEL BIOCARE REPLACE NP	33.390.805.01-2	1,7	90	0,7	8	0,65	3	50
	33.490.805.01-2	1,7	90	0,7	8	0,65	4	50
	33.690.805.01-2	1,7	90	0,7	8	0,65	6	50

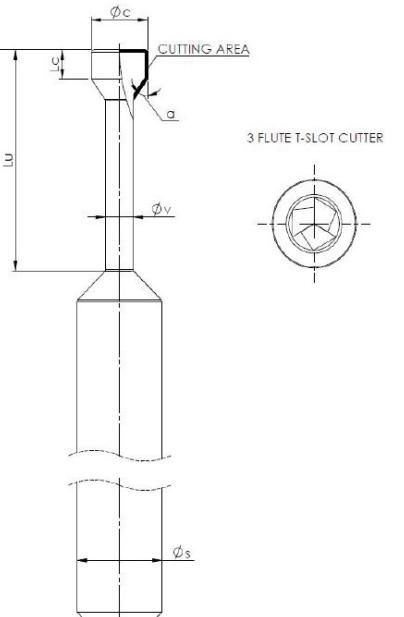

MAIN COMPATIBILITY	REFERENCE	CUTTING DIAMETER	SEAT	CUTTING LENGTH	USEFUL LENGTH (max. drilling depth)	STEM CUTTING DIAMETER	SUPPORT DIAMETER (SHANK)	TOTAL LENGTH
		\varnothing_c	Lc	Lu	\varnothing_v	\varnothing_s	Lt	
BEGO S/RI 3,25-3,75/4,1/4,5/5,50	33.335.676.01-2	1,8	35	1	6,7	0,9	3	50
	33.435.676.01-2	1,8	35	1	6,7	0,9	4	50
	33.635.676.01-2	1,8	35	1	6,7	0,9	6	50
KLOCKNER ESSENTIAL CONE 4,5 KLOCKNER ESSENTIAL CONE 4,5 OCTACONE 12° KLOCKNER ESSENTIAL CONE 4,5 OCTACONE 25° KLOCKNER VEGA RV XIVE S 3,8/4,5	33.345.856.01-2	1,8	45	1	8,5	0,9	3	50
	33.445.856.01-2	1,8	45	1	8,5	0,9	4	50
	33.645.856.01-2	1,8	45	1	8,5	0,9	6	50
MIS C1 RP/WP S&M OUTLINK 3,3/4,1 S&M PREMIUM KHONO 3,3/3,8/4,25	33.360.756.01-2	1,8	60	1	7,5	0,9	3	50
	33.460.756.01-2	1,8	60	1	7,5	0,9	4	50
	33.660.756.01-2	1,8	60	1	7,5	0,9	6	50
ASTRA EVOLUTION UNIT ABUTMENT ZIMMER SCREWVENT 3,5 ZIMMER SCREWVENT 4,5 ZIMMER SCREW VENT 5,7	33.370.716.01-2	1,8	70	1	7,1	0,9	3	50
	33.470.716.01-2	1,8	70	1	7,1	0,9	4	50
	33.670.716.01-2	1,8	70	1	7,1	0,9	6	50
ANTHOGYR MULTIUNIT 4,8 BIOMET 3I OSSEOTITE NP/WP BTI EXTERNAL CONNECTION NP/RP/WP BTI MULTI-H UNIVERSAL RP KEYSTONE PRIMA NP/RP/WP MIS MULTI-UNIT ST NEOSS PROACTIVE 3,4/4,1 NOBEL BIOCARE BRANEMARK RP NOBEL BIOCARE MULTI-UNIT RP	33.390.716.01-2	1,8	90	1	7,1	0,9	3	50
	33.490.716.01-2	1,8	90	1	7,1	0,9	4	50
	33.690.716.01-2	1,8	90	1	7,1	0,9	6	50
STRAUMANN INTERNAL OCTAGON 4,8 STRAUMANN INTERNAL OCTAGON 6,5	33.315.708.01-2	2	15	1	7	1	3	50
	33.415.708.01-2	2	15	1	7	1	4	50
	33.615.708.01-2	2	15	1	7	1	6	50
STRAUMANN SYNOCTA RP	33.330.708.01-2	2	30	1	7	1	3	50
	33.430.708.01-2	2	30	1	7	1	4	50
	33.630.708.01-2	2	30	1	7	1	6	50
NOBEL BIOCARE ACTIVE RP NOBEL BIOCARE ACTIVE WP	33.335.758.01-2	2	35	1	7,5	1	3	50
	33.435.758.01-2	2	35	1	7,5	1	4	50
	33.635.758.01-2	2	35	1	7,5	1	6	50
OSSTEM IMPLANT TS RP	33.345.808.01-2	2	45	1	8	1	3	50
	33.445.808.01-2	2	45	1	8	1	4	50
	33.645.808.01-2	2	45	1	8	1	6	50
ASTRA EVOLUTION 4,8/5,4 ASTRA LILAC NOBEL BIOCARE BRANEMARK WP NOBEL BIOCARE REPLACE RP/WP/6,0	33.390.958.01-2	2	90	1	9,5	1	3	50
	33.490.958.01-2	2	90	1	9,5	1	4	50
	33.690.958.01-2	2	90	1	9,5	1	6	50



TALLADIUM GUARANTEE

TERMS AND CONDITIONS

These guarantee terms and conditions ("T&C") cover the entire range of Talladium products ("Products"), manufactured by TALLADIUM ESPAÑA S.L. and distributed by Geoda Medical S.L. or official dealers. The guarantee described in these T&C is exclusively in benefit of the clinician ("Clinician") and of the dental technician ("Technician") and not for the benefit of third parties or institutions, including patients.

GUARANTEE PERIOD

TALLADIUM ESPAÑA S.L. offers a lifelong guarantee for its entire range of products starting from the date of issue of the invoice.

GUARANTEE SCOPE

Subject to the limitations and exceptions described in these T&C, TALLADIUM ESPAÑA S.L. will offer the following benefits:

QUALITY: If there are defects in the materials or in the manufacturing of the Product, TALLADIUM ESPAÑA S.L. will replace the Product with no additional cost.

SAFETY: If, having complied with all the product indications, the prosthesis should have to be made again, due to a fault in the Dynamic Abutment® or Dynamic Titanium Base® system, TALLADIUM ESPAÑA S.L. will replace the abutments and screws necessary to remake the prosthesis, as well as the costs derived from its manufacturing.

In case of having used our products and having complied with all the product indications, the implants suffer any damage, TALLADIUM ESPAÑA S.L. will pay the cost of the implants. This coverage will only be valid during the first 6 months after the collocation of the prosthesis which includes our products.

CLAIM REQUIREMENTS AND PROCEDURE

To receive the benefits indicated in these T&C, the treating Clinician must satisfy the following requirements:

- a) The claim must be notified to TALLADIUM ESPAÑA S.L. within (30) days since the date the claimed defect was detected.
- b) This requires that the Clinician or Technician must contact the customer service department by telephone or by e-mail to make the claim.
- c) A claim form will be completed, which, together with a document or report which justifies the faulty Product and the faulty Product itself, will be sent by the customer to TALLADIUM ESPAÑA S.L. offices, within the previously indicated period.
- d) Clinicians or Technicians presenting a claim in agreement with these T&C must be up to date in any payments owing to TALLADIUM ESPAÑA S.L. or to any of its subsidiaries, at the time when the claim form is presented.
- e) All the use procedures of our Products must be carried out in agreement with the instructions of TALLADIUM ESPAÑA S.L. as well as in accordance with commonly accepted dentistry practices.
- f) The expenses derived from this procedure will be assumed by the customer. The return shipping costs will be assumed by TALLADIUM ESPAÑA S.L. in all those cases covered by these T&C.

Regardless of the guarantee rights, claims should be notified as soon as possible in order to comply with regulatory requirements.

GENERAL LIMITATIONS OF THIS GUARANTEE

With the exception of the guarantee described in these T&C, neither TALLADIUM ESPAÑA S.L. nor its representatives, nor third parties manufacturing or distributing the Products, represent or offer a guarantee, agreement or any other express or implicit, oral or written, commitment, with respect to the Products (without limitation), including guarantees involved in the marketing, durability or suitability for individual uses or purposes.

In addition and within the maximum extent permitted by the relative law, TALLADIUM ESPAÑA S.L. rejects (on its own behalf, and on behalf of its representatives and third parties that manufacture or distribute Products) any responsibility with respect to any direct or indirect damage caused, which may result from or be a consequence of the design, composition of the dental prosthesis into which the Products are integrated.

GUARANTEE EXCLUSIONS

TALLADIUM ESPAÑA S.L. limits this guarantee to:

- Transformed abutments that form part of the dental prosthesis. But not the screws used to anchor them.
- Clinical screws that have been in the mouth for more than 2 years.

AMENDMENT OR SUSPENSION OF THE GUARANTEE

TALLADIUM ESPAÑA S.L. reserves the right to amend or withdraw these T&C at any time and without prior notification. Any modification or suspension shall not affect products already placed in patients.

Ed.2019-01



ALCALDE MONTANYA, 17 · 25005 · LLEIDA (SPAIN)

INTERNATIONAL +34 973 289 580

das@dynamicabutment.com

SPAIN +34 973 289 580

spain@dynamicabutment.com

www.dynamicabutment.com



ED.2019-8



ALCALDE MONTANYA, 17
25005 · LLEIDA (SPAIN)

INTERNATIONAL +34 873 450 709
das@dynamicabutment.com

SPAIN +34 973 289 580
spain@dynamicabutment.com

www.dynamicabutment.com